



WatchPAT™ 200 Unified

Operation Manual

Itamar Medical **REF** OM2196331



R^xonly Caution: Federal law restricts this device to sale by or on the order of a licensed healthcare practitioner

Copyright © 2002 - 2020 By **Itamar Medical Ltd.**
WatchPAT™ and **PAT®** are trademarks of **Itamar Medical, Ltd.**

This manual and the information contained herein are confidential and are the sole property of  **Itamar Medical Ltd.** Only **Itamar Medical Ltd.** or its licensees have the right to use this information. Any unauthorized use, disclosure or reproduction is a direct violation of **Itamar Medical's** proprietary rights.

DISCLAIMER

Itamar Medical Ltd. shall not be held responsible in any manner for any bodily injury and/or property damage arising from operation or use of this WatchPAT™200 Unified other than that which adheres strictly to the instructions and safety precautions contained herein and in all supplements hereto and according to the terms of the warranty provided in the License Agreement in Appendix C.

Itamar Medical Ltd.
9 Halamish St., P.O. Box 3579
Caesarea Ind. Park, 3088900, Israel
Tel: International + 972-4-617-7000, US 1-888-7ITAMAR
Fax + 972 4 627 5598
www.itamar-medical.com

This product and/or method of use, is covered by one or more of the following US patents: 6319205, 6322515, 6461305, 6488633, 6916289, 6939304, 7374540, as well as any pending US patent applications and corresponding patents and/or applications filed in other countries.



EN ISO 13485:2016

See appendix D for contact information of the regulatory authorized representative

Record of Editions

Edition	Date	Description	Chapter	Pages
1 (based on OM2196330 ed. 9)	August 2013	Standards, Preparing for use, Specifications table and minor wording changes. Update for bracelet and multi-night support. Updated for uPAT probe.	All	All
2	July 2014	Insert note Added WatchPAT™ Updating pictures Updating intended use Updating exclusion criteria Updating Standards Updating symbols/labels Attaching uPAT probe Medes and Itamar's addresses Adding Training Resources appendix	-, All All 1.1 1.3 1.6 1.11,1.12 7.3 -, App. D App.H	ii All All 1 2 3-4 7-8 35 i, 58, 59 65
3	September 2014	Specifications table: Update Arms limit	10	42
4	Oct–Nov 2014	Updating Caution and Warning symbols Adding MDD, CE mark and EC rep. symbol Updating Manufacturing Declarations Adding cross reference Adding spare parts list	All -,1.5, 1.7, 1.11, 1.12 App.F 2.1 App.I	All i, 2, 4, 7, 8 60-63 10 68
5	March 2015	Updating Manufacturing Declaration Table 2	App. F	61
7	July 2015	Add FDA #K to section 1.13 Adding MDD to list of standards	1.13 1.6	8 4
8	June 2016	ARMS – correcting typo Updating company zip code Updating company logo Updating - Symbols Used on the Product Labels, adding WEEE symbol Updating Manufacturing Declarations	App.G - 1.11 App.F	64, 66 - 8 60
9	September 2016	Update Intended Use Update restrictions for use Update exclusion criteria Add pediatric use section Update data generated by the WatchPAT00U Update standards	1.1 1.2 1.3 1.4 1.5	1 1,2 2 2 3

		Update French translation of Safety Precautions	1.7	4
		Update FDA clearance #	1.11	7
		Update Patient test		
		Update Packing the carrying case	1.14	9
		Update maintenance instructions to include routine maintenance	2.4.3	17
		Update applying the WP	3.9	23
		Update patient training guidelines	6	29-33
		Add note under SBP accuracy	7	34,36
		Update address	8	40,41,42
			App. A	50
			App. C	60
10	May 2017	Update Rx caution	-	-
		Updated intended use to include AHIC	1.1	1
		Update data generated by the WP200U	1.5	3
		Update Company & product Standards	i,1.7	-,4-5
		Added note regarding Central+	1.9	5
		Update symbols	1.12	8-9
		Update labels	1.13	9
		Update FDA clearance #	1.14	9
		Update SBP section to include RESBP data	4.1,App A	25, 48-49
		Update Tamper-Proof bracelet photos (new design)	4.2,App B	26,54-55
		Added instructions when using SBP/RESBP sensor	7.1, 8.3, App A	36, 42, 48
		Update specification table to include RESBP, update recording time and updating Probe's transportation Temp.	10	47
		Updating Manufacturing Declarations	App. F	64-68
		Added App H	App. H	72
		Added RESBP when referring to snoring and BP sensor	All	All
		Update photos to include the RESBP sensor	All	All

11	Jan 2018	Updating CE marking with the accompanying BSI notified body number 0086 Updating Intertek certification marks Deleting information in App I Adding zzzPAT HW requirements and information regarding Manual	-,1.12, 1.13 -, App.H	i, 8-9 iii, 74
12	March 2019	Updating CE marking with the new notified body number 2797 Updating standards	-,1.12 all	i,8 all
13	Sep 2019	Update Standards Update Tamper-Proof Bracelet instructions Update EU REP address	1.7 4.2 App D	4 29 63
14	Jan 2020	Added warning for double night	4.3	30
15	Feb 2020	Add restriction for AHIC Changed from Exclusion Criteria to Precautions Change Precautions wording for arrhythmias	1.2 1.3 1.3	2 2 2
16	Sep 2020	Remove CE Mark, explanation and classification related to MDD Updating device label	1.6, 1.7 1.11, 1.12	i, 3, 5 8-9

Note:

- Latest version of the WatchPAT™ system Operation Manual is available at:

<http://www.itamar-medical.com/Support/Downloads.html>
- zzzPAT Software Manual is also available on the zzzPAT installation CD and is installed as part of the software installation.

Printed copy will be provided within 7 calendar days if requested at no additional cost.

Table of Contents

1	GENERAL INFORMATION	1
1.1	Intended Use / Indications for Use	1
1.2	Restrictions for Use	1
1.3	Precautions	2
1.4	Additional Precautions specific to pediatric use	2
1.5	Data Generated by the WatchPAT™ 200U	3
1.6	Quality Assurance System: EN ISO 13485.....	4
1.7	CSA Compliance	5
1.8	Conventions Used in this Manual.....	5
1.9	Warnings, Cautions and Notes	6
1.10	Safety Precautions.....	7
1.11	Symbols Used on the Product Labels.....	8
1.12	WatchPAT™ 200U Device Labels	9
1.13	FDA information.....	9
2	OVERVIEW	10
2.1	System Description.....	11
2.2	User Interaction with the WatchPAT™ Device Keys.....	13
2.3	WatchPAT™ Device Function	14
2.4	Built-In Self-Diagnostic Procedures	17
3	PREPARATION FOR SLEEP STUDY	21
3.1	Charging the Battery.....	21
3.2	Preparing the Snore and Body Position Sensor	22
3.3	Preparing the Wrist Strap.....	22
3.4	Mounting the WatchPAT™ on the Wrist Strap	23
3.5	Replacing the uPAT Probe	23
3.6	Preparing the WatchPAT™ Device for a New Study	24
3.7	Testing the WatchPAT™ Device	24
3.8	WP200U Self-diagnostic Test Results and Trouble-shooting	24
3.9	Packing the Carrying Case.....	25
4	OPTIONAL FUNCTIONS	26
4.1	Using the integrated Snore & Body Position Sensor.....	26
4.2	Tamper-Proof Testing with WatchPAT™ Device.....	27
4.3	Multi-night study	30
5	DATA DOWNLOAD AND ANALYSIS	31
6	MAINTENANCE	32
6.1	Cleaning.....	33

6.2	Handling.....	34
6.3	Replacing the uPAT Probe Cable	34
6.4	Replacing the Battery	35
6.5	Setting the Time and Date of the WatchPAT™ device.....	36
6.6	Storing the WatchPAT™ device.....	36
7	APPLYING THE WATCHPAT™ DEVICE	37
7.1	Preparing for Use of the WatchPAT™ Device	37
7.2	Applying the WatchPAT™ Device	38
7.3	Attaching the uPAT Probe.....	39
7.4	Switching On the WatchPAT™ device	40
7.5	When You Wake Up	41
7.6	Important Notes.....	42
8	PATIENT TRAINING – GUIDELINES	43
8.1	Walk Through the Process of Using the WatchPAT™ device.....	43
8.2	Product Introduction.....	43
8.3	Applying the WatchPAT™ device.....	43
8.4	Switching on the WatchPAT™ Device	44
8.5	Removing the WatchPAT™ Device	44
8.6	Patient Training.....	44
8.7	Review Safety, General and Functional Issues	45
9	TROUBLESHOOTING GUIDE.....	46
9.1	Operator Error Messages	46
9.2	Patient Error Messages	47
10	SPECIFICATIONS	48
	APPENDIX A: WATCHPAT™ INTEGRATED SNORING + BODY POSITIONING SENSOR OPERATING INSTRUCTIONS (SBP/RESBP)	49
	APPENDIX B: TAMPER-PROOF TESTING WITH WATCHPAT™..	55
	APPENDIX C: LICENSE AGREEMENT	57
	APPENDIX D: REGULATORY REPRESENTATIVE.....	63
	APPENDIX E: DESCRIPTION OF THE WATCHPAT™200U UPAT PROBE.....	64
	APPENDIX F: MANUFACTURING DECLARATIONS ACCORDING TO IEC 60601-1 & 60601-1-2.....	65
	APPENDIX G: SPO2 ACCURACY IN THE WATCHPAT™200U	70

APPENDIX H: WP200U EFFECTIVENESS IN DETECTING CENTRAL SLEEP APNEA SYNDROME USING A THRESHOLD OF AHIC=10	73
APPENDIX I: ZZZPAT HARDWARE REQUIREMENTS	74
APPENDIX J: SPARE PARTS LIST	75

List of Figures

Figure 1 – Packed Device	12
Figure 2 – WatchPAT™ 200U Device with Sensors.....	12
Figure 3 – The Buttons and Display	13
Figure 4 – Service Ports and Peripherals.....	14
Figure 5 – WatchPAT™ Wrist Strap.....	14
Figure 6 – Charging the WatchPAT™ Device	21
Figure 7 – Disconnecting the Probe	23
Figure 8 – Probe Disconnected.....	23
Figure 9 – WatchPAT™ Fully Prepared	24
Figure 10 – WatchPAT™ Device with Tamper-Proof Bracelet.....	27
Figure 11 – Bracelet on Patient's Hand	27
Figure 12 – WatchPAT™ Device with Cable for Bracelet.....	29
Figure 13 – WatchPAT™ Device with Bracelet	29
Figure 14 – Bracelet and WatchPAT™ Device on a Patient's Hand.....	29
Figure 15 – Cut the Bracelet	29
Figure 16 – Case for 3 Night Multi-night Study.....	30
Figure 17 – uPAT Probe Cable with Screw.....	34
Figure 18 – Replacing the uPAT Probe	35
Figure 19 – Replacing the Battery.....	36
Figure 20 – Finger Designation	38
Figure 21 – Putting On The Wrist Strap.....	38
Figure 22 – Wearing the WatchPAT™ Device	38
Figure 23 – Placing Finger In uPAT Probe	39
Figure 24 – Removing TOP Tab	39
Figure 25 – Wearing the WatchPAT™ – Ready for Sleep.....	40

List of Tables

Table 1 – Operator Troubleshooting.....	46
Table 2 – Patient Troubleshooting.....	47
Table 3 – WatchPAT™ 200U Specifications.....	48

1 GENERAL INFORMATION

This manual is part of the WatchPAT™200 Unified system.

1.1 Intended Use / Indications for Use

The WatchPAT™200U (WP200U) device is a non-invasive home care device for use with patients suspected to have sleep related breathing disorders. The WP200U is a diagnostic aid for the detection of sleep related breathing disorders, sleep staging (Rapid Eye Movement (REM) Sleep, Light Sleep, Deep Sleep and Wake), snoring level and body position. The WP200U generates a peripheral arterial tonometry ("PAT") Respiratory Disturbance Index ("PRDI"), Apnea-Hypopnea index ("PAHI"), Central Apnea-Hypopnea index ("PAHIc"), PAT sleep staging identification (PSTAGES) and optional snoring level and body position discrete states from an external integrated snoring and body position sensor. The WP200U's PSTAGES and snoring level and body position provide supplemental information to its PRDI/PAHI/PAHIc. The WP200U's PSTAGES and snoring level and body position are not intended to be used as the sole or primary basis for diagnosing any sleep related breathing disorder, prescribing treatment, or determining whether additional diagnostic assessment is warranted.

PAHIc is indicated for use in patients 17 years and older. All other parameters are indicated for 12 years and older.

1.2 Restrictions for Use

1. The WP200U should be used only in accordance with physician's instructions. For precautions see Section 1.3.
2. Only qualified medical personnel may authorize the use of the WP200U.
3. Qualified medical personnel must instruct the patients (and accompanying individual if needed) how to attach and use the WP200U prior to use.
4. In the event of equipment malfunction all repairs should be executed by authorized Itamar Medical Ltd. personnel or licensed service agents.
5. The eligibility of a patient for a PAT® study is entirely at the discretion of a physician, and is generally based upon the patient's medical status.
6. The WP200U system in whole, or in part, may not be modified in any way.
7. The WP200U is used as an aid for diagnostic purposes only, and should not be used for monitoring.
8. Only suitably trained and qualified personnel should be authorized to prepare the WP200U equipment prior to use.
9. The WP200U Operation Manual should be carefully studied by the authorized operators, and kept where it is easily accessible. Periodic review of the Manual is recommended.
10. Itamar Medical Ltd. makes no representation whatsoever, that the act of reading the Manual renders the reader qualified to operate, test or calibrate the system.
11. The tracings and calculations provided by the WP200U system are intended as tools for the competent diagnostician. They are explicitly not to be regarded as a sole incontrovertible basis for clinical diagnosis.

-
12. In the event that the system does not operate properly, or if it fails to respond to the controls in the manner described in this Manual, the operator should refer to the Troubleshooting section. If necessary, contact our service office to report the incident, and to receive further instructions.
 13. The step by step instructions for the patient should be carefully followed when attaching the unit to the patient.
 14. The WP200U is not indicated for patient with injuries, deformities or abnormalities that may prevent proper application of the WP200U device.
 15. The WP200U is not indicated for children less than 12 years old.
 16. The AHIC was not clinically assessed for patients who are in high altitudes or for patients using opioids.

1.3 Precautions

The WatchPAT™200U should not be used in the following cases:

1. Use of one of the following medications: alpha blockers, short acting nitrates (less than 3 hours before the study).
2. Permanent pacemaker: atrial pacing or VVI without sinus rhythm.
3. Sustained* non-sinus cardiac arrhythmias.
** In the setting of sustained arrhythmia the WatchPAT's automated algorithm might exclude some periods of time, resulting in a reduced valid sleep time. A minimum valid sleep time of 90 minutes is required for an automated report generation.*
4. The WP200U is not indicated for children who weigh less than 65 lbs.

1.4 Additional Precautions specific to pediatric use

The WatchPAT™200U is indicated for use in patients 12 years and above.

The following Precautions and Notes are referring to pediatric aged 12-17 years.

Precautions:

1. Pediatric patients with severe comorbidities such as Down syndrome, neuromuscular disease, underlying lung disease or obesity hypoventilation should be considered for sleep study in a laboratory polysomnograph (PSG) rather than a home sleep testing (HST).
2. It is recommended that the physician makes sure that the patient and his/her guardian are aware that the use of specific drugs and other substances used to treat ADHA, antidepressants, corticosteroids, anticonvulsants, use of caffeine, nicotine, alcohol and other stimulants might interfere with sleep and affect the sleep study's conditions.

Notes:

1. PAT Respiratory Disturbance Index (PRDI) is indicated for patients 17 years of age or greater
2. The snoring and body position safety and effectiveness was not validated on pediatric patients

-
3. Special attention on training the pediatric patient and / or his accompanying individual on use and placement of the device prior to initiating a sleep study with the WatchPAT™ device (for further details see section 7 and section 8)

1.5 Data Generated by the WatchPAT™200U

The WatchPAT™200U generates a PAT respiratory disturbance index (“PRDI”) , PAT Apnea-Hypopnea Index (“PAHI”), PAT central Apnea-Hypopnea Index (pAHIC), percentage of total sleep time with Cheyne-Stokes Respiration pattern (%CSR) and PAT sleep staging identification (“PSTAGES”). The WP200U respiratory indices and sleep stages are estimates of conventional values and stages identification that are produced by polysomnography (“PSG”). The WatchPAT™200U also generates optional acoustic decibel detector used for snoring level and body position discrete states from an external integrated snoring and body position (SBP/RESBP) sensor.

PRDI is indicated for patients 17 years of age or greater.

1.6 Quality Assurance System: EN ISO 13485

The Itamar Medical WP200U is compliant to the following standards.

	STANDARD	#
1.	Medical electrical equipment – Part 1: General requirements for basic safety and essential performance	IEC 60601-1:2005 + CORR.1:2006 + CORR.2:2007 + AMI:2012 ANSI/AAMI ES60601-1:2005/(R) 2012 and A1:2012, C1:2009/(R) 2012 and A2:2010/(R) 2012 CAN/CSA -C22.2 No.60601-1 :08
2.	Medical electrical equipment – Part 1-2: General requirements for basic safety and essential performance - Collateral standard: Electromagnetic compatibility - Requirements and tests	IEC 60601-1-2:2014
3.	Medical Device Software – Software Life Cycle Processes	IEC 62304 : 2006 + AMD1:2015
4.	Medical electrical equipment -- Part 1-11: General requirements for basic safety and essential performance -- Collateral standard: Requirements for medical electrical equipment and medical electrical systems used in the home healthcare environment	IEC 60601-1-11:2015
	Degrees of protection provided by enclosures (IP Code) – IP22	IEC 60529 Ed 2.1:2001
5.	Medical devices - Application of usability engineering to medical devices	IEC 62366:2007 + A1:2014
6.	Medical electrical equipment - Part 1-6: General requirements for basic safety and essential performance - Collateral standard: Usability	IEC 60601-1-6:2010 + A1:2013
7.	Medical devices. Application of risk management to medical devices	EN ISO 14971:2012
8.	Medical devices. Symbols to be used with medical device labels, labelling and information to be supplied. General requirements	ISO 15223-1:2016
10.	Graphical symbols for electrical equipment in medical practice	IEC TR 60878:2015
11.	Graphical symbols - Safety colours and safety signs -- Registered safety signs; refer to instruction manual/ booklet	ISO 7010:2011 (M002)
12.	Information supplied by the manufacture with medical devices	EN 1041:2008 + A1:2013
13.	Biological evaluation of medical devices - Part 1: Evaluation and testing	ISO 10993-1:2009
14.	Medical electrical equipment - Part 2-61: Particular requirements for basic safety and essential performance of pulse oximeter equipment	ISO 80601-2-61:2011

	STANDARD	#
15.	FDA Quality Systems Regulation (QSR)	21 CFR part 820
16.	Medical devices. Quality management systems. Requirements for regulatory purposes	EN ISO 13485:2016

1.7 CSA Compliance



The product is certified by CSA.

1.8 Conventions Used in this Manual


Note: Throughout this document, the references WatchPAT™, WatchPAT™200U and WP200U device are used to refer to the WatchPAT™200 Unified device.

Note: Throughout this document, the reference Snore & Body Position sensor is referring to both SBP sensor and RESBP sensor unless specified otherwise.

Note: Central+ is a WatchPAT™ module that enables identification of central apnea. Central+ functionality can be achieved when using the WatchPAT™ with the RESBP sensor and compatible software.

	<p>Warnings are used to identify conditions or actions, which - if the instructions are ignored - may violate patient safety, or cause damage/malfunction to the system, resulting in non recoverable loss of data.</p> <p>Les avertissements sont utilisés pour identifier les conditions ou les actions qui- si elles sont ignorées- peuvent porter atteinte à la sécurité des patients ou causer des dommages au système et résulter à une perte irréversible des données.</p>
--	---

	<p>Cautions are used to identify conditions or actions, which could cause interference with data acquisition and/or impair study results.</p> <p>Les précautions sont utilisées afin d'identifier les conditions ou les actions qui peuvent interférer avec le ramassage de données et provoquer des résultats équivoque.</p>
---	---

	<p>Notes are used to identify an explanation, or to provide additional information for purposes of clarification.</p> <p>Les notes sont utilisées pour identifier les explications et pour donner des informations supplémentaires dans le but de clarifier.</p>
---	--

1.9 Warnings, Cautions and Notes

The WP200U is internally powered from a 4.2 V battery.

The WP200U is portable with continuous operation.

The WP200U uses BF patient applied parts.

The WP200U uses UL listed power supply (USA & Canada only).

The power supply is used in a non-patient environment only.

The WP200U should only be transported in its original case.

There are no serviceable parts inside the WP200U.

Environmental conditions during transportation & storage: See Specifications section.

Environmental conditions during operation: See Specifications section.

Sleep professionals (other than patients) using the WP200U should read the Operation Manual.

1.10 Safety Precautions

	<p>WARNINGS</p> <p>Use only the AC adapter provided (5V DC, 5W maximum capacity power supply). Only authorized personnel may charge the WP200U. Failure to heed this warning may cause permanent damage to the equipment.</p> <p>Do not let the unit get wet.</p> <p>Avoid placing food or water on any part of the system.</p> <p>In the event of fire use only fire extinguishers approved for use on electrical fires.</p> <p>Handle unit with care. This unit is sensitive to extreme movements and to falling.</p> <p>Do not attempt to connect or disconnect any part of the unit.</p> <p>Do not try to introduce any foreign object into the unit.</p> <p>The WP200U MUST be charged ONLY after being removed from the patient!</p> <p>The WP200U MUST be removed from the patient BEFORE connecting it to a PC!</p>
	<p>AVERTISSEMENTS</p> <p>Utiliser uniquement l'adaptateur CA fourni avec le dispositif (5V DC, 5W alimentation maximale). Seuls les techniciens autorisés peuvent recharger le dispositif WP200U. Cet avertissement est essentiel pour éviter des dommages irréparables à l'équipement.</p> <p>Ne pas mouiller l'unité.</p> <p>Éloigner le dispositif de toute source d'eau ou nourriture.</p> <p>En cas d'incendie, utiliser uniquement des extincteurs homologués pour l'utilisation en cas d'un incendie dû à une source électrique.</p> <p>Manier avec précaution. L'unité est fragile : éviter les mouvements soudains et chute.</p> <p>Ne pas tenter de brancher ou débrancher une des parties de l'unité.</p> <p>Ne pas introduire un corps étranger à l'intérieur de l'unité.</p> <p>Le système WP200U doit être rechargé uniquement après avoir été détaché de la main du patient.</p> <p>Il est impératif de détacher le système WP200U de la main du patient avant de le relier à l'ordinateur.</p>

1.11 Symbols Used on the Product Labels

	Follow instructions for use
	Type BF applied part
	The product is certified by CSA
	Date of manufacture
3.7V DC 	Battery Operating Voltage
	Single use, do not re-use
	Temperature limit
	Use-by date
	Medical device Manufacturer
	Catalogue Number
	Serial Number
IP22	Ingress protection The device is protected against insertion of fingers and vertically dripping water shall have no harmful effect when the device is tilted at an angle up to 15° from its normal position

<div style="display: flex; justify-content: space-around; border: 1px solid black; padding: 2px;"> EC REP </div>	Authorized representative in the European Community
	Caution: Federal law restricts this device to sale by or on the order of a licensed healthcare practitioner
	According to the WEEE Directive 2012/19/EU, all waste electrical and electronic equipment (EEE) should be collected separately and not disposed of with regular household waste. Please dispose this product and all of its parts in a responsible and environmentally friendly way.

1.12 WatchPAT™200U Device Labels



Located on WatchPAT™200U device



Located on WatchPAT™200U device

1.13 FDA information

The WatchPAT200U is cleared by the FDA under K161579, trade name Watch-PAT 200U (WP200U).

2 OVERVIEW

Obstructive sleep apnea syndrome (OSAS) is considered a major public health problem. The prevalence of the syndrome is estimated at 2% to 5% in the adult population. It is characterized by recurrent events of complete or partial obstruction of the upper airways during sleep, often leading to hypoxemia, and/or arousals associated with sympathetic nervous system activation. The diagnosis and assessment of the sleep apnea patient is based on the Respiratory Disturbance Index (RDI), the number of Apneas, Hypopneas and Respiratory Effort Related Arousals (RERA) per hour of sleep, along with sleep architecture. The common consequences of this sleep disruption are daytime sleepiness, poor daytime performance and increased vulnerability to accidents. Cardiovascular complications such as systemic/pulmonary hypertension, ischemic heart disease and arrhythmias are the major sequel of OSAS in the adult population.

The WP200U is worn on the wrist and is utilizing a plethysmographic based finger-mounted probe that measures the PAT[®] (Peripheral Arterial Tone) signal. The PAT[®] signal is a measurement of the pulsatile volume changes in the fingertip arteries which reflects the relative state of the arterial vasomotor activity, and thus indirectly the level of sympathetic activation. Peripheral arterial vasoconstriction, which mirrors sympathetic activation, is shown as attenuation in the PAT[®] signal amplitude.

The same probe measures RED and IR channels used for the measurement of SpO₂ signal. The PAT[®] and SpO₂ signals are recorded continuously and stored on an embedded micro SD card, together with data from a built-in actigraph (embedded in the WP200U). Snoring and Body Position signals are generated from the SBP/RESBP integrated sensor (optional). The RESBP (Respiratory Effort Snoring and Body Position) sensor records the subject's chest movement signal in addition to the snoring and body position signals that are included with the SBP sensor.

Following the sleep study, the recordings are automatically downloaded and analyzed in an offline procedure using the proprietary zzzPAT software.

The zzzPAT algorithms use the four WP200U channels (PAT[®], Pulse Rate, Oxygen saturation and actigraphy) for the detection of sleep related breathing disorders and sleep staging (Rapid Eye Movement (REM), Light Sleep, Deep Sleep and Wake). In WP200U only, for further identification of central apnea the respiratory movement channel generated from the RESBP sensor is used in the zzzPAT algorithm in addition to the other channels. The zzzPAT uses WP200U's snoring and body position channels to generate snoring level and body position discrete states. The use of SBP/RESBP is optional and according to physician preference.

The software issues comprehensive reports of the study, with statistics and graphic presentation of the results. The whole night data can be viewed and the automatically detected events can be revised manually.

2.1 System Description

The WP200U system is comprised of the following items:

- WP200U device that includes:
 - Embedded actigraph
 - Embedded pulse oximeter
 - Embedded CPU and electrical circuit card
 - Embedded micro SD card drive
 - Rechargeable Lithium Ion Battery
 - LCD display
- uPAT probe (includes oximetry)
- uPAT probe connection cable
- Wrist Strap
- Snore and Body Position sensor (SBP/RESBP) – optional
- Cable for Tamper-Proof Bracelet – optional
- Tamper-Proof Bracelet - optional
- AC adapter
- USB cable
- Step-by-Step Reference Guide (to be used in conjunction with Section 7)
- Quick Reference Cards (to be used in conjunction with Section 8)
- Carrying case



Figure 1 – Packed Device



Figure 2 – WatchPAT™200U Device with Sensors

An additional item required for the operation of the system is the zzzPAT kit. zzzPAT is a proprietary PC software for initializing the study, retrieving, analyzing and displaying the data. For more information, refer to the zzzPAT Operation Manual.

2.2 User Interaction with the WatchPAT™ Device Keys

The WatchPAT™ has the following keys (see Figure 3):

- Central On/Enter key to power on the WatchPAT™ (the only key visible to the patient)
- Outer ring containing four keys (left, right, up, down) that may be used by the Operator for entering the diagnostic mode and navigating through the diagnostic menu. These keys are hidden from the patient.



Figure 3 – The Buttons and Display

LCD Display

The display is used for reading status and error messages. The display is divided to three sections: Title, Info and Status.

- Title (first line): Current operational mode and time
 - PATIENT mode while recording night study
 - DIAGNOSTIC mode while testing device
 - PC HOST while connecting to PC
 - CHARGER mode while connecting to AC adapter
- Info (2nd-5th line): Specific information depending on operational mode
- Status (last line): Message indicating device status depending on operational mode

Service Ports and Peripherals

The WatchPAT™ device has 4 ports that are used either for sensor connections or for servicing and charging (see Figure 4).

-
- The bracelet port is used for connecting the tamper-proof bracelet.
 - The uPAT probe port is used for connecting the uPAT probe
 - A port for connecting the optional Snore & Body Position sensor
 - The USB port is used for charging or connecting to the PC



Figure 4 – Service Ports and Peripherals

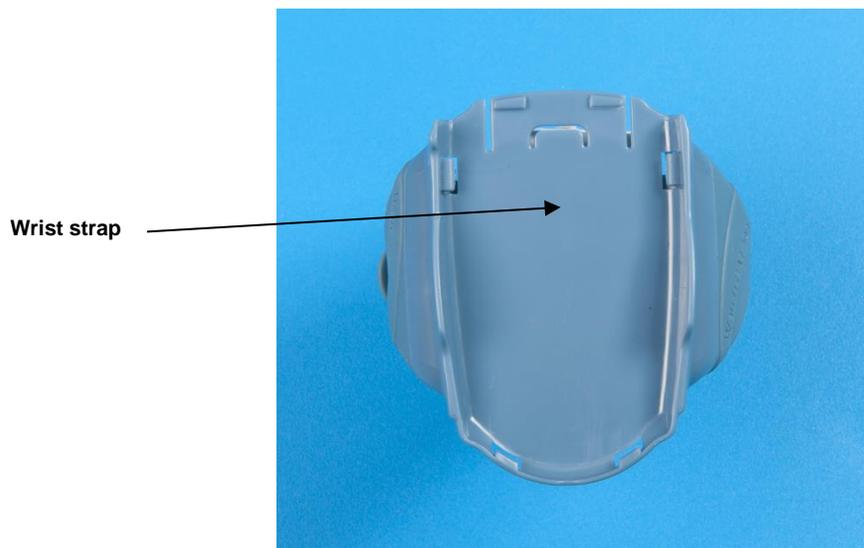


Figure 5 – WatchPAT™ Wrist Strap

2.3 WatchPAT™ Device Function

The WatchPAT™ records the following channels:

- PAT® Signal

-
- Oxygen saturation
 - Actigraphy (movement)
 - Acoustic decibel detector for Snoring evaluation (optional)
 - Body Position (optional)
 - Chest movement signal (optional)

The overnight sleep study data is stored on an embedded micro SD card in the WatchPAT™ device. After the study is recorded, the data is downloaded from the WatchPAT™ device through the USB cable using the zzzPAT software. The zzzPAT software, utilizing automatic algorithms, detects respiratory and other events that occurred during sleep as well as periods of REM, deep sleep, light sleep and wakefulness. The pulse rate signal is derived from the PAT® signal and used in the automatic analysis. The software issues comprehensive detailed reports of the study. The whole night data can be viewed on the PC screen and the automatically detected events can be revised manually.

An optional tamper-proof patient identification function is available using a custom bracelet whose presence during the night verifies that the identified patient is indeed the one sleeping with the device (see

Tamper-Proof Testing with WatchPAT™ Device section).

The patient normally sleeps only one night with the WatchPAT™ device unless an optional multi-night option is selected which enables an up to 3 nights study with the same device (see

Multi-night study section).

2.4 Built-In Self-Diagnostic Procedures

2.4.1 Operator Tests

The WatchPAT™200 unified contains a comprehensive built-in self-diagnostic procedure. This procedure is available to the operator and hidden from the patient. The procedure can be accessed if the UP and DOWN keys (see Figure 3) are pressed simultaneously after the device is powered ON (during the first 30 seconds only after the device is powered ON).

The procedure performs the following test:

- Device Test – tests the WatchPAT™ for errors before performing a night study (make sure all sensors are connected before initiating this test)

	<p style="text-align: center;">Note</p> <p>In all times, the current time is shown in the upper right hand corner of the LCD display.</p>
---	--

To run the self-diagnostic procedure:

- Press the ENTER button (Center key) for 2 seconds till the Itamar medical logo appears on the LCD screen
- Immediately press the **UP + DOWN** keys (see Figure 3) simultaneously for 1 second

The following screen will be displayed:

```
DIAGNOSTIC      22:40
2.2140         20-Jul-08
*device test (30001)

  end testing
Select test ↑↓
```

- First line displays title and current time
- Second line displays current embedded S/W version (2.2139) and current date
- Third line displays option for running device test (serial number of device in parenthesis)
- Fifth line indicates option for end testing (turn device off). If no test is selected within 3 minutes the WatchPAT™ device will automatically shut down
- The Up, Down keys (↑↓) navigate between the lines.

- An asterisk will indicate current selection. When moving the ↑↓ keys, the asterisk will move to indicate the current selection. Press the central Enter key to make the desired selection.

It is recommended that you perform the Device every time you prepare the WatchPAT™ for a night study.

2.4.2 Device Test

At the completion of the device test, a **TEST PASSED** indicates that the device is ready for the night study.

```

DEVICE TEST      22:50
  ID=111-11-1111
  sbp=missing

<-Back
TEST PASSED      2:54

```

At the completion of the device test, a **TEST FAILED** indicates a problem that should be taken care of before the device is released for a night study.

```

DEVICE TEST      22:50
  ID=111-11-1111
  pat=missing

<-Back          More->
TEST FAILED      2:54

```

The following are the possible error, warning or information messages:

- File error: not loaded, missing – the study file was not loaded or somehow the file was deleted
- File error: used x/3 x=1..3 – only when multi-night option is selected
- Battery error: low – needs charging
- Probe error: used, missing, bad – connect an unused probe
- Hardware (H/W) error: error code - contact customer support
- SBP/RESBP (Snore and Body Position sensor) warning: sensor missing – does not affect PASSED status
- RTC (Real Time Clock) warning: faulty – indicates problem with internal clock but does not affect PASSED status
- Bracelet error: missing – the study file was chosen with the bracelet option but the bracelet is not connected during the device test
- Information messages:
 - multi-night=on - when a multi night study is required

-
- bracelet=on - when a study with tamper-proof patient identification bracelet is required

More-> indicates that there are more error/warning messages and will be displayed if the Right (->) button is pressed.

<-Back will move to the previous screen if the Left (<-) button is pressed.


2.4.3 Patient Test

When the patient (and accompanying individual if needed) turns on the WatchPAT™ device by pushing the On/Enter key (center button) for about 2 seconds a self-diagnostic test is automatically performed and the following screen is displayed:

```
PATIENT                22:51  
  
Please wait  
Testing...
```

If the WatchPAT™ device passes this self-diagnostic test, the following screen will be displayed:

```
PATIENT                22:51  
  
GOOD NIGHT!!!  
  
Time elapsed=9:50  
Recording...
```



Note

During recording the LCD display turns off to conserve battery life. Any key pressed during Recording will turn on the LCD for 30 seconds.

If the WatchPAT™ device fails this self-diagnostic test, the following screen will be displayed:

```
PATIENT                22:51  
Error=xxxx  
Device S/N=xxxxxx  
  
Call Help Desk  
TEST ABORTED
```

-
- The error message will be displayed for 1 minute and then the WatchPAT™ device will shut off.
 - If this is a study with the tamper-proof bracelet and the wrong bracelet is connected the "wrong bracelet" error message appears.
 - If this is study with the tamper-proof bracelet and the bracelet is not connected the "connect bracelet" error message appears in order to remind the patient to connect the bracelet.

The following are the possible error/warning messages:

xxx1 - battery low

xx2x – uPAT probe error (used probe)

xx4x – File error (no new file)

xx8x - uPAT probe error (bad probe)

x4xx – SBP/RESBP missing warning

	<p style="text-align: center;">Note</p> <p>The "x" stands for 0-F value (Hexadecimal code)</p> <p>Error codes are additive, i.e. both uPAT probe and File errors will produce error code xx6x.</p>
--	---

3 PREPARATION FOR SLEEP STUDY

3.1 Charging the Battery

The battery must be charged every time the WatchPAT™ device is prepared for use. The battery may be charged using the AC adapter provided.

To charge the WatchPAT™ device:

1. Gently slide the WatchPAT™ device out of the wrist strap until a click is heard and the USB port is exposed.
2. Connect the USB port of the WatchPAT™ device to the AC adapter provided (see Figure 6).

	Warning
For charging use only an AC adapter having a 5V DC output, with 5W minimum capacity. Using any other AC adapter may cause permanent damage to the WatchPAT™ and may jeopardize the operator.	



Figure 6 – Charging the WatchPAT™ Device

3. The LCD will blink slowly and the following screen will be displayed:

CHARGER	22:51
Bat=3.12 V	
Charging...	

-
- The display will show “**CHARGER**” if you are charging with the AC adapter or “**PC HOST**” if you are charging with a computer.
 - The current battery voltage is shown.
 - Charge the battery the first time for approximately three hours. Thereafter recharging takes approximately 1-1.5 hours.
4. When charging is complete, the LCD will stop blinking and the following screen will be displayed:

CHARGER	22:51
Bat=4.2 V	
Charging complete	

5. Disconnect the AC adapter or communication cable. The WatchPAT™ device will switch off in 30 seconds.
6. Reseat the WatchPAT™ device in the wrist strap by gently sliding it back in until a click is heard.

Should a charging error arise the LCD will blink rapidly and the following screen will be displayed.

CHARGER	22:51
Bat=4.2 V	
Charger fault	

3.2 Preparing the Snore and Body Position Sensor

Attach the small round double sided adhesive sticker to the Snore and Body Position sensor on the back side (front side has an image), by peeling off the cover on one side of the sticker.

For more details see Appendix A: WatchPAT™ Integrated snoring + Body Positioning Sensor Operating Instructions (SBP/RESBP)

3.3 Preparing the Wrist Strap

The wrist strap requires no special preparation other than ensuring its cleanliness. You may clean it if needed. See section 6.1 for detailed cleaning instructions.

3.4 Mounting the WatchPAT™ on the Wrist Strap

To mount the WatchPAT™ device on the wrist strap:

Gently slide the WatchPAT™ device into the wrist strap until a click is heard indicating that it is properly seated.

3.5 Replacing the uPAT Probe

	<p style="text-align: center;">Warning</p> <p>The uPAT probe connector is very sensitive and therefore should never be left exposed. Keep the connector connected to the probe at all times, especially during cleaning. Replace the probe just before performing the Device test.</p>
---	--

Remove a used probe by pressing the small tab (clip) marked by the arrow in Figure 7, and then, holding the connector's slider, gently slide it away from the probe – do not pull the slider off by pulling the cord, as it may damage the wiring. Properly dispose of used probes.



Figure 7 – Disconnecting the Probe

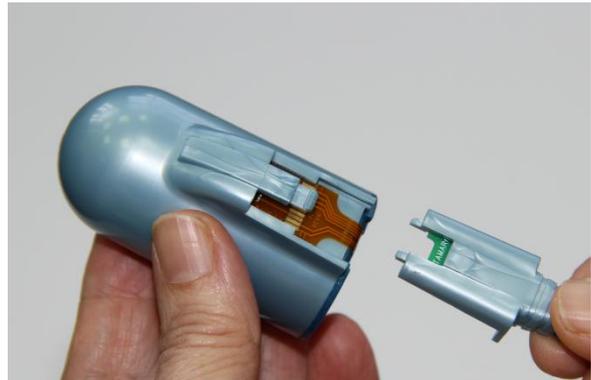


Figure 8 – Probe Disconnected

Connect a new probe by inserting the blue slider to the probe until the blue tab of the probe clicks into its place.

	<p style="text-align: center;">Note</p> <p>Take care when inserting the blue slider to insure proper seating in the probe.</p>
---	---



Figure 9 – WatchPAT™ Fully Prepared

3.6 Preparing the WatchPAT™ Device for a New Study

Refer to the zzzPAT Software Manual for preparation of the WP200U for a new study.

3.7 Testing the WatchPAT™ Device

Run the built-in self-diagnostic facility as described in Section 2.4 above.

The WatchPAT™ device is now ready for performance of a sleep study by the patient (Figure 9).


3.8 WP200U Self-diagnostic Test Results and Trouble-shooting

Should any of the self-diagnostic tests fail or report error messages refer to the trouble-shooting guide in Section 9.

3.9 Packing the Carrying Case

The following items must be placed inside the carrying case, in their respective compartments (see Figure 1 – Packed Device):

- The WatchPAT™ device mounted in the Wrist strap with the uPAT probe attached.
- Step-by-Step Reference Guide to the WatchPAT™ device.
- Body Position and Snore sensor (optional)
- Cable for bracelet (optional for patient identification)
- 2 extra uPAT probes and AC adapter (optional for multi-night)



Note

Demonstrating the use of the WatchPAT™ device to the patient (and accompanying individual if needed) is important for obtaining reliable recordings and improving patient confidence.

4 OPTIONAL FUNCTIONS

4.1 Using the integrated Snore & Body Position Sensor

The integrated sensor consists internally of two sensors: a snore sensor and a body position sensor.



A - Integrated SBP sensor



SBP Sensor Attachment



B - Integrated RESBP sensor



RESBP Sensor Attachment

The integrated sensor is powered by the WatchPAT™ device and does not require a battery. It is automatically activated by the WatchPAT™ device when plugged into the Snore & Body position port.

The **snore sensor** is an acoustic decibel detector. It uses a very sensitive microphone that responds to snoring and other sounds in the audio range and converts them to a small analog voltage that provides a clear, reliable indication of the presence of these sounds.

The **body position** sensor uses a 3-axis accelerometer that provides a signal directly proportional to the patient's sleeping posture (supine, prone, right, left and sit).

For RESBP only: The **chest movement signal** uses the same 3-axis accelerometer to provide raw chest movement signal data for measuring subject's breathing during the night. See Appendix A: WatchPAT™ Integrated snoring + Body Positioning Sensor Operating Instructions (SBP/RESBP).

4.2 Tamper-Proof Testing with WatchPAT™ Device

The WatchPAT™ device Tamper-Proof bracelet is an add-on accessory used to authenticate the patient doing a sleep study and assure the study is recorded from the right person.

The bracelet is a single use small plastic band designed to be worn around the wrist of the hand. It contains an electronic circuit that signals to the WatchPAT™ device the integrity of the bracelet and a unique identification. During the night the bracelet is connected to the WatchPAT™ device using a small cable (see Figure 10).

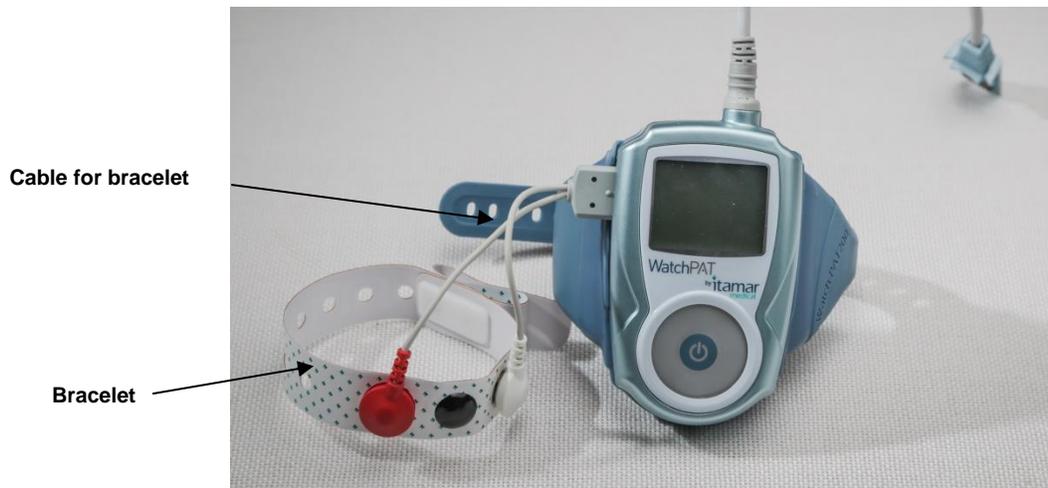


Figure 10 – WatchPAT™ Device with Tamper-Proof Bracelet

Before the device is given to the patient for home sleep study, the technician identifies the patient and secures the bracelet to the patient's wrist by a tamper-proof connector that ensures the bracelet will not be removed without cutting the Bracelet.



Figure 11 – Bracelet on Patient's Hand

When preparing the WatchPAT™ device for a sleep study, the technician pairs the Tamper-Proof Bracelet and the device and registers the bracelet's unique ID in the WatchPAT™ device (see Appendix B: Tamper-proof testing with WatchPAT™)

	WatchPAT™ 200U	Action	Comment
Important Note	Important Note	This short guide will instruct a WatchPAT trained operator on how to perform Tamper-Proof testing with the WatchPAT. For complete WatchPAT training and instructions please refer to the WatchPAT user manual and to the zzzPAT user manual.	<ul style="list-style-type: none"> • Make sure the zzzPAT version is: 4.4.64 or higher • Make sure the WatchPAT embedded software version is: 3.2217 or higher • Make sure you enable the "Tamper-Proof Testing" option from the zzzPAT "Setup" menu > "General Settings"
Study Preparation	1 New Study on zzzPAT	While preparing the new study on the zzzPAT (refer to the user manual for detailed instructions), check the box "Study with Tamper-Proof Testing" at the bottom of the "New Study" screen. Note: Once you enable this option you MUST use a bracelet for the night study. The WatchPAT will NOT function without a bracelet connected to it.	
Bracelet Preparation	2 Bracelet	Select a Tamper-Proof Bracelet for the study.	
Bracelet Preparation	3 Connecting the Cable to the WatchPAT	Connect the gray cable with the red and white snap buttons to the WatchPAT socket.	
Bracelet Preparation	4 Connecting the Bracelet	Connect the red and white snap buttons to the red and white snaps on the bracelet respectively.	

The patient can wear the Bracelet for several days, continuing normal day-to-day activity until he is ready to record his sleep study. Before starting the recording, the patient will need to connect the Bracelet, via the bracelet's cable 2 connectors, to the WatchPAT™ device. The device will not start without connection to the paired Bracelet.



Figure 12 – WatchPAT™ Device with Cable for Bracelet



Figure 13 – WatchPAT™ Device with Bracelet



Figure 14 – Bracelet and WatchPAT™ Device on a Patient's Hand

During the recording the device will periodically check the Bracelet connectivity. The recording will be stopped if the connection to the Bracelet will be lost for the time exceeding a predefined limit.

After the recording is completed the patient can cut the Bracelet and return it with the device for study analysis.



Figure 15 – Cut the Bracelet

4.3 Multi-night study

A patient study may be defined as multi-night study and the patient can sleep up to 3 nights with the same WatchPAT™ device. The multi-night option may be selected during New Study function (see zzzPAT Operation Manual).

If a 3 night multi-night option is selected the patient must replace the uPAT probe and charge the device between nights. Two extra uPAT probes and a WatchPAT™ device AC adapter must be added to the WatchPAT™ device case.

If a 2 night multi-night option is selected the patient must replace the uPAT probe only after the first night without the need to charge the device between nights. One extra uPAT probe must be added to the WatchPAT™ device case.

	<p style="text-align: center;">Warning</p> <p>If your WP200U contains the Semicom 423048A-SL011/ITMR battery (Itamar REF AS0037060), in order to ensure that the WP200U will provide 2 eight hours nights, the WP200U must be charged longer. A period of approximately 4 hours charging (with the provided AC/DC adapter) must be applied. In this case, the “charging complete” indication on the LCD applies only for a single night charging and is not applicable for a two night study. See Replacing the Battery section for inspecting the battery type inside the device.</p>
---	--

In case of multi-night study all of the patient studies will be loaded automatically to the zzzPAT during the upload (see zzzPAT Operation Manual).

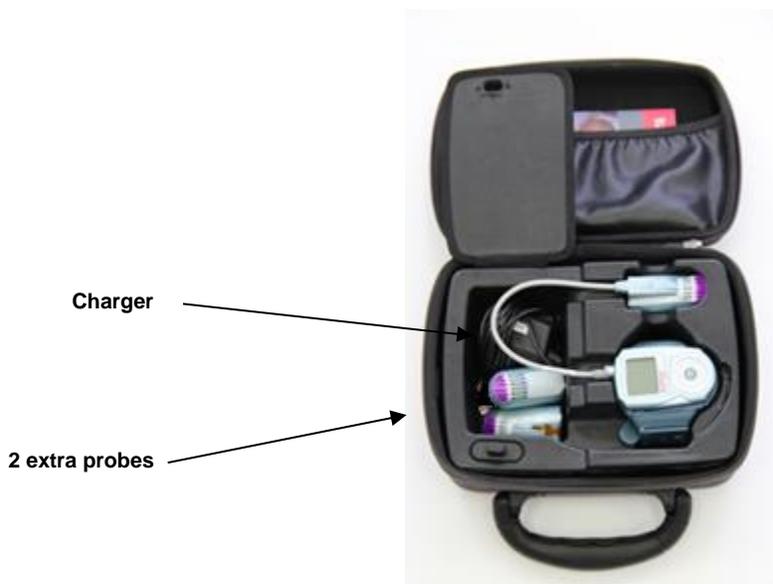


Figure 16 – Case for 3 Night Multi-night Study

5 DATA DOWNLOAD AND ANALYSIS

Following the sleep study the WatchPAT™ device is returned to the referring sleep clinic for data downloading and analysis by the zzzPAT software.

To download and analyze the study data:

1. Connect the USB port of the WatchPAT™ device to the computer (see Figure 4) The WatchPAT™ device will switch off and then switch on in charging mode.
2. Activate the zzzPAT software to download and analyze the study data.

See the zzzPAT Software User Manual for detailed instructions.

6 MAINTENANCE

The WatchPAT™ device has been designed and manufactured to meet all safety requirements applicable to medical equipment. To ensure maximum safety of operation, the system should be used and maintained in strict compliance with the safety precautions, warnings and operating instructions provided in this Manual.

In order to prevent unnecessary failures while patient is using the device, we recommend performing the routine maintenance recommendations as well as the preventive maintenance recommendations as described in this section.

Routine maintenance recommendations

- a) Cleaning the device, wrist strap and SBP sensor.
- b) Device should be inspected for possible defects, in the device, cables and sensors. The product must be serviced on any case of damage.
- c) PAT cable's electrical connectors should be visually inspected while replacing a probe. The product should be serviced in case any damage to the connector is found.
- d) The following items should be visually inspected and replaced if found damaged: strap, carrying case and all accessories.
- e) Complete technician test must be done and passed with no errors prior to handing the product to a patient.
- f) The product should be stored in its carrying case while not in use or charged.

Preventive maintenance recommendations

- a) Battery – replace battery after 200 sleep studies, after 1 year or when charging time, using the provided power supply, exceeds 2.5 hours.
- b) PAT Cable – replace the PAT cable after 200 sleep studies, after 1 year or when it is found broken on any of its components.
- c) SBP Sensor – replace if its connector is broken, if the cable near the connector is peeling off or if it is found broken on any of its components.

See sections 6.1,6.2, 6.3 and 6.4 below for detailed instruction on Cleaning and replacing the uPAT cable and the battery respectively.

Following is a summary table with routine and preventive maintenance recommendations:

Routine maintenance recommendations:

Routine maintenance action	Scenario	
	Back from sleep study	Handing to patient
Cleaning	X	
Check cable connections	X	
Check carrying case	X	X
Check strap	X	X

Perform technician test		X
--------------------------------	--	---

Preventive maintenance recommendations:

Routine maintenance action	Scenario	
	Lesser of: 200 studies, 1 year, error message in device test	When a defect is found or upon error message
Replace battery	X	
Replace PAT cable	X	X
Replace SBP sensor		X
Replace strap		X
Replace charger		X
Replace carrying case		X

Other system parts are not user-serviceable parts. Any maintenance needs that are not listed here should be performed only by qualified service personnel, authorized by Itamar Medical Ltd.

6.1 Cleaning

The various components of the WatchPAT™ device have different cleaning requirements:

- The WatchPAT™ device
- The wrist strap
- The Snore & Body Position sensor

6.1.1 Cleaning the WatchPAT™ Device

In order to clean the WatchPAT™ device proceed as follows:

- Wipe parts with a clean, dry, lint-free cloth.
- Clean casing with lint free cloth lightly moistened with 70% ethyl alcohol or isopropyl alcohol (IPA).

	Warning Clean the WatchPAT™ device only with the uPAT probe attached.
---	---

6.1.2 Cleaning the Wrist Strap

You may clean the wrist strap with lint free cloth lightly moistened with 70% ethyl alcohol or isopropyl alcohol (IPA).

In order to disinfect the wrist strap by immersing into disinfecting liquid follow the steps:

-
- Remove WatchPAT™ device from wrist strap
 - Immerse wrist strap in 70% ethyl alcohol or isopropyl alcohol (IPA)

6.1.3 The uPAT Probe

The uPAT probe is designed for a single use only. It may not be cleaned and must be discarded and replaced before each study.

6.1.4 The Snore & Body Position Sensor

Using 70% ethyl alcohol, thoroughly clean both sensor and cable.

6.2 Handling

Handle with care:

- Use only the designated case for transportation
- Store at room temperature, and avoid direct sun light
- Do not expose the WatchPAT™ device to extreme temperature or humidity conditions (such as storing in a car or bathroom)

6.3 Replacing the uPAT Probe Cable

To replace the uPAT probe cable:

1. Carefully disconnect the uPAT probe cable from the WatchPAT™ device. Make sure you remove the screw prior to disconnecting the uPAT cable.



Figure 17 – uPAT Probe Cable with Screw

2. Connect a new uPAT probe cable by gently inserting the connector into the WatchPAT™ device. Make sure you secure back the screw.



Figure 18 – Replacing the uPAT Probe



Warning

Use only the original screw that belongs to the WatchPAT™ device. Using different screw could harm the device.

6.4 Replacing the Battery



Warning

Replace the battery only with an authorized battery provided by Itamar Medical Ltd.

In the event of a battery error message during the self-diagnostic tests or after charging, it may be necessary to replace the battery.

To replace the battery:

1. Open the battery compartment cover with a Phillips screwdriver.
2. Gently open the battery connector by disconnecting the 2 parts (you will need to remove the transparent tape that secures the battery connector closed).
3. Remove the battery.
4. Insert the new battery into the battery compartment.

-
5. Insert the 3 pin connector into the corresponding battery connector (one pin is longer so it may properly be inserted in only one direction). Secure the battery connector closed with a small piece of transparent tape.
 6. Close the battery compartment cover and secure back the screw.

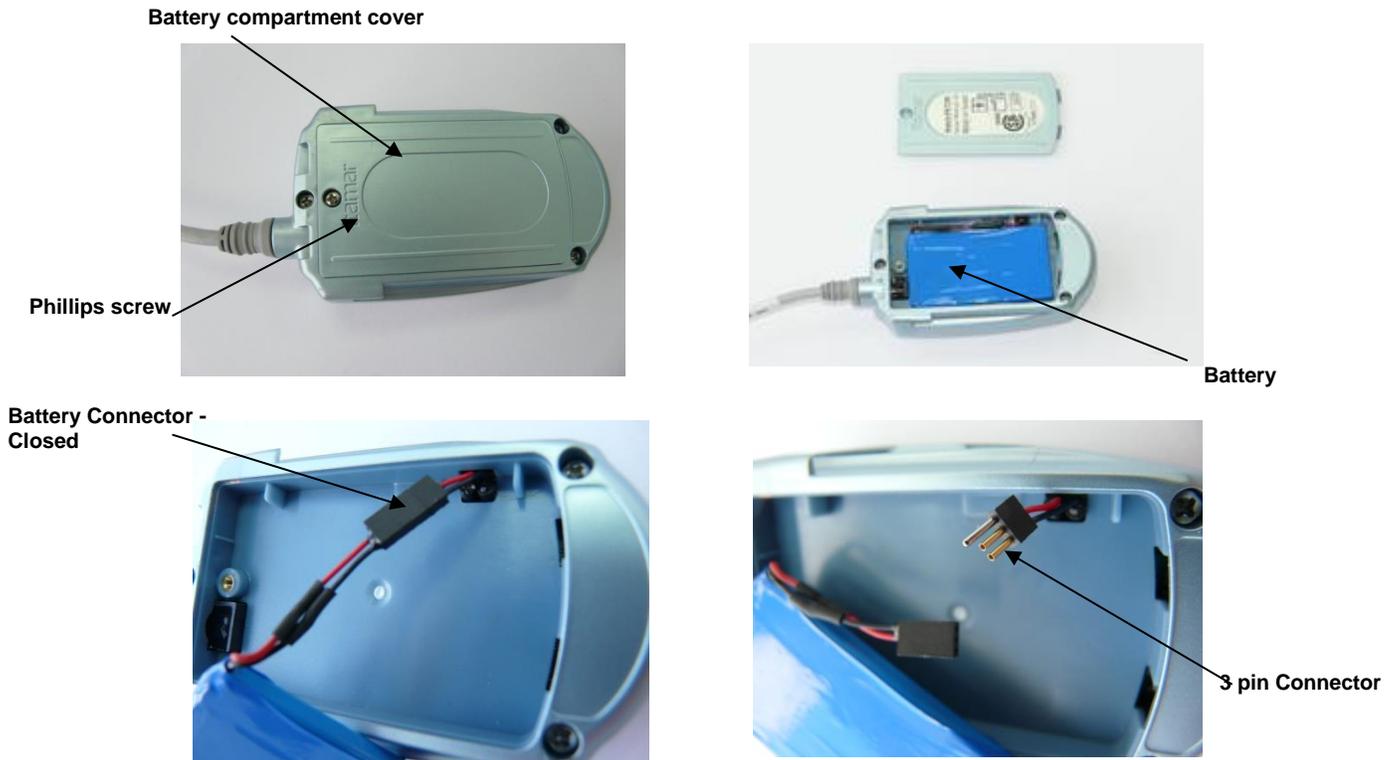


Figure 19 – Replacing the Battery


6.5 Setting the Time and Date of the WatchPAT™ device


The WatchPAT™ device Time and Date can be set through the zzzPAT application. Refer to the zzzPAT Software Manual for preparation of the WatchPAT™ device for a new study.

6.6 Storing the WatchPAT™ device

- The WatchPAT™ device should be stored in its carrying case at room temperature and low humidity.
- In order to preserve battery performance when the WatchPAT™ device is not in use, store with the battery fully discharged.
- Before storing the WatchPAT™ device allow it to deplete the battery charge until it shuts down automatically.

7 APPLYING THE WATCHPAT™ DEVICE

	<p style="text-align: center;">Note</p> <p>These instructions are designed to help the patient use the WP200U after seeing a demonstration by trained personnel of how to mount the probes on his/her fingers and correctly operate the WatchPAT™ device.</p>
---	---

	<p style="text-align: center;">Note</p> <p>In the case of pediatric patient, special attention on training the patient and / or his accompanying individual on use and placement of the device prior to initiating a sleep study with the WatchPAT™ device.</p>
---	--

The following detailed instructions are summarized in the patient's step-by-step reference guide. They are written as if the reader is the patient using the WatchPAT™ device.

7.1 Preparing for Use of the WatchPAT™ Device

Before using the WP200U, review the following notes:

- Remove tight clothing, rings, watches and jewelry from your non-dominant hand and wrist and from your neck and chest.
- We recommend that the uPAT probe be attached to the index finger of your non-dominant hand (Figure 20). The following instructions relate specifically to this finger. Patients with very large fingers may use their small finger (pinky) for the uPAT Probe.
- Ensure that fingernail of finger that will be monitored are well trimmed, (less than 1mm from nail bed) with no jagged edges. Clip and file nail, if necessary.
- Remove artificial fingernail or dark nail polish from the monitored finger.
- If you are using the SBP/RESBP sensor, trim chest hair to ensure the sensor attached directly to your skin.
- You may need some assistance putting on the WatchPAT™ device. If needed have someone present to assist you.
- Make sure the room you are sleeping in is as quiet as possible during the night, turn off any possible noise sources. When using the Snore & Body Position sensor it is advised to sleep alone in the room.

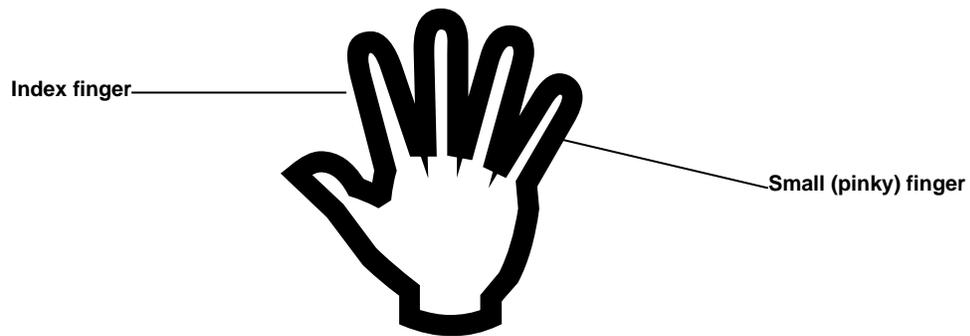


Figure 20 – Finger Designation

7.2 Applying the WatchPAT™ Device

To apply the WatchPAT™ device to your wrist:

1. Open the carrying case and take out the wrist strap with the WatchPAT™ device mounted. All parts should already be connected, as illustrated in Figure 9.
2. Ensure that the WatchPAT™ device is firmly seated in the wrist strap. If not, gently seat the WatchPAT™ device in the strap by sliding it into its seating position. You will hear a click when the WatchPAT™ device is properly seated in the strap.
3. Place the wrist strap with the WatchPAT™ device on the non-dominant arm and close it snugly but not tightly. Ensure that the rounded end is towards the body and the open end towards the fingers. You may find it convenient to place the wrist strap with the WatchPAT™ device face down on the table and then place the back of the wrist over the wrist strap in order to fasten the straps (Figure 21).
4. At this point the uPAT probe is hanging loose (Figure 22Figure 22 – Wearing the WatchPAT™ Device).



Figure 21 – Putting On The Wrist Strap


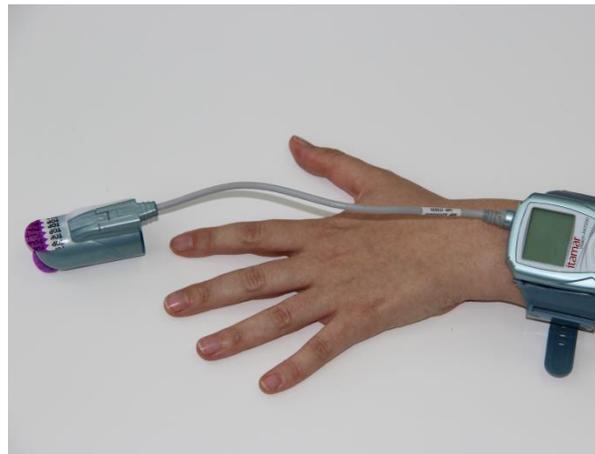


Figure 22 – Wearing the WatchPAT™ Device

7.3 Attaching the uPAT Probe

Proper probe placement is critical for good performance.



Note

The tab inside the probe should be removed only **AFTER** the finger is inserted into the probe.

To attach the uPAT probe:

1. Insert your index finger (or other if so instructed) gently into the probe until it reaches the end (see Figure 23 –).
2. Make sure that the paper tab marked TOP is above your nail.
3. Detach and gradually remove the tab marked TOP slowly and firmly while pressing the tip of probe against a hard surface (WatchPAT™ case, table, etc.) until the tab is completely removed from the probe (Figure 24). You might feel a slight suction once the tab is removed. For small fingers secure the probe to the finger with a medical tape.

The uPAT probe is now attached (Figure 25).




Figure 23 – Placing Finger In uPAT Probe



Figure 24 – Removing TOP Tab




Figure 25 – Wearing the WatchPAT™ – Ready for Sleep



Note

DO NOT remove the uPAT probe before the night study is terminated. Once the probe is removed it cannot be re-attached.



Note

If the Snore & Body position sensor is included in the WatchPAT™ device case see Appendix A: WatchPAT™ Integrated snoring + Body Positioning Sensor Operating Instructions (SBP/RESBP)

7.4 Switching On the WatchPAT™ device


You are now ready to switch on the WatchPAT™ device.

Just before you lie down to go to sleep, firmly press the ON/Enter center button (Figure 3) until the LCD display lights up. After a short delay the LCD will display “Good Night! Recording...”

```
PATIENT      22:51

GOOD NIGHT!!!

Time elapsed=9:50
Recording...
```




Note

To conserve the battery the LCD display will switch off after a few seconds. Pressing any button will restore the display for about 30 seconds.

7.5 When You Wake Up

When you awake, remove the WatchPAT™ device from your arm as follows:

1. Remove both probes from your fingers.
2. Take off the wrist strap.
3. Place all parts in the carrying case.



Note

Pressing the center button does not switch off the WatchPAT™ device. Approximately ten hours after the WatchPAT™ device is turned on, it will switch off. This is normal.

7.6 Important Notes


Wearing the WatchPAT™ device should not cause any discomfort or pain. If you experience wrist or arm discomfort, loosen up the wrist strap. If the discomfort is not alleviated immediately, call the service number.

- Do not attempt to connect or disconnect any part of the unit.
- Do not try to introduce any foreign object into the unit.
- Do not try to connect the unit to an electrical supply or any other unit, machine or computer.
- If any part appears disconnected or does not resemble the illustrations, call the service number for assistance.
- Do not, under any circumstances, attempt to fix the problem yourself.

If you have any questions about using the machine, before, during or after your at-home recording session, call the service number.

8 PATIENT TRAINING – GUIDELINES

Instruct the patients (and accompanying individual if needed) how to attach and use the WP200U prior to use.



Note

In the case of pediatric patient, special attention on training the patient and / or his accompanying individual on use and placement of the device prior to initiating a sleep study with the WatchPAT™ device.

8.1 Walk Through the Process of Using the WatchPAT™ device

- Product introduction – WatchPAT™ device, wrist strap, uPAT probe
- WatchPAT™ device and wrist strap attachment
- Probe and sensor attachment
- Switch on
- Ending the study

8.2 Product Introduction

- Open the Demo-case and introduce the ‘Quick guide step-by-step’ instruction manual.
- Introduce each component by its name and identify it as in the figures in the manual.

8.3 Applying the WatchPAT™ device

Use the Demo Kit.

- Demonstrate how to apply the WatchPAT™ device on your wrist while following the ‘step by step’ guidelines and referring to the relevant figures.
- Demonstrate the following:

1. Hand Preparation

- Remove rings, watches and jewelry from hand
- Remove fingernail polish and artificial nails
- Make sure index finger nail is closely trimmed

2. Attaching the Snore & Body Position Sensor (optional)

- The sensor is attached to the patient’s chest right under the sternal notch. The sternal notch is the little U shape where the collar bones meet at the top of the breast bone.

-
- If needed, trim chest hair to ensure the sensor attached directly to your skin.
 - To position the sensor attach it with the image standing up (cable pointing down) after peeling off the round adhesive sticker and pressing against the skin.
 - Make sure the sensor is tight against the skin.
 - Secure the snoring sensor in place with medical tape.

3. Wearing the Wrist Strap

- Should be comfortable, not too tight.

4. Attaching the WatchPAT™ Device

- Make sure the WatchPAT™ device is properly mounted on the wrist strap. If it is loose, gently slide it in until you hear a click.

5. Attaching the uPAT Probe

- Insert finger all of the way into the probe
- Press tip of probe against a hard surface (WatchPAT™ device case, table, etc.) while removing tabs in order to keep the finger from moving inside the probe
- Remove the Tab by pulling slowly and gradually
- For small fingers secure the probe to the finger with a medical tape.
- The probe is limited to a SINGLE USE. Do not remove probe during the night.

8.4 Switching on the WatchPAT™ Device

- Demonstrate switching on the WatchPAT™ device by pressing the round center button
- Push button firmly until the LCD display lights up

8.5 Removing the WatchPAT™ Device

- Demonstrate how to remove the WatchPAT™ device and place it back in the carrying case.
- The WatchPAT™ device doesn't switch off – once turned on it will record until the battery is exhausted.

8.6 Patient Training

-
- Following your demonstration have the patient attach the demo device by himself or with the assistance of accompanying individual if needed.
 - Verify that the attachment is properly done.

8.7 Review Safety, General and Functional Issues

- Avoid exposing the WatchPAT™ device to extreme conditions (high temperature, high humidity)
- Provide a telephone number to call in case of questions or problems.

9 TROUBLESHOOTING GUIDE

9.1 Operator Error Messages

If an error message is displayed while performing the self-diagnostic tests, take the actions specified below. If the problem persists contact Itamar or an authorized representative.

Table 1 – Operator Troubleshooting

Error	Possible Reason	Action
File error		
Not loaded	Study not initialized for new patient	Connect device to PC and perform New Study in zzzPAT
Battery error % full	Battery defective or uncharged	Charge battery or replace
Probe error		
Used	Probe previously used	Replace probe
Missing	Probe absent	Attach probe
Bad	Probe is defective	Replace probe
Hardware status error code	WatchPAT™ device defective	Consult Itamar or authorized representative
SBP/RESBP disconnected even if it is connected	WatchPAT™ device or SBP/RESBP sensor defective	Consult Itamar or authorized representative
RTC faulty	WatchPAT™ device defective	Consult Itamar or authorized representative
Short recording time	Patient removed the WP200U or probe from hand prematurely	Explain proper use to patient
	Insufficient battery charge caused early termination of recording	Recharge battery and try again
	Damaged WatchPAT™ device	Contact your authorized sales representative

9.2 Patient Error Messages

If an error message is displayed when the patient powers on the WatchPAT™ device, the patient should take the actions specified below. If the problem persists the patient may contact Itamar or an authorized representative directly.

Table 2 – Patient Troubleshooting

Error	Possible Reason	Action
WatchPAT™ device doesn't switch on	ON button not activated	Press the ON button firmly for at least 3 seconds
	uPAT probe not connected	Ensure probe is connected and try again
Probe disconnected	Probe may not be connected, or may be a used probe	Check connection of probe to cable and cable to the WatchPAT™ device; check if probe has been previously used and replace with new probe if necessary
Hardware code	WatchPAT™ device failure	Contact Itamar or authorized representative

10 SPECIFICATIONS

Table 3 – WatchPAT™200U Specifications

Properties		Description
uPAT Probe		Itamar's proprietary probe. Measures PAT and Oximetry.
Recording Time		Approx. 10 hours
Channels		Measuring 4-7 signals: PAT, Pulse rate, Oximetry, Actigraphy, Snoring (optional), Body Position (optional), Chest Movement (optional)
Sample Resolution		PAT and Actigraph – 12 bit, oximetry – 1% Snoring – 12 bit, Chest Movements – 12bit x 3 axes, Body Position – 5 discrete states
User Interface		LCD display
Oximetry		Arms \leq 3% (in range 70%-100%)
Accuracy	<i>Pulse rate</i> <i>Amplitude</i>	30-150 \pm 1 bpm 0-0.5V \pm 10%
PAT Channel	<i>Bandwidth</i>	0.1-10 Hz
Data Storage	<i>Media</i>	Micro SD card
	<i>Capacity</i>	64 MB (minimum)
	<i>Format type</i>	Formatted to FAT 32
Power Supply	<i>Battery</i>	Proprietary, rechargeable Lithium Ion Battery
	<i>Capacity</i>	> 500-700 mAh
	<i>Cell Type</i>	Lithium Ion cell type
	<i>Internal Charger</i>	Proprietary Lithium Ion battery charger
	<i>External Power Supply</i>	5V DC, 5W with USB connector
Operating Voltage		3.3 V
Temperature	<i>Operation</i>	0°C to 40 °C
	<i>Storage (Device)</i>	-20°C to 40 °C
	<i>Transport (Device & Probe)</i>	-20°C to 60 °C
	<i>Storage (Probe)</i>	0°C to 40 °C
Humidity	<i>Operating</i>	10% – 93% (non-condensing)
	<i>Storage & Transport</i>	0% – 93% (non-condensing)
Atmospheric pressure	<i>Operating & Storage</i>	10 – 15 psi
	<i>Transport</i>	8 – 15 psi
Dimensions	<i>L x W x H</i>	80 x 50 x 20 mm
	<i>Weight</i>	130 gr (excluding uPAT probe weight of 20 gr)


APPENDIX A: WatchPAT™ Integrated snoring + Body Positioning Sensor Operating Instructions (SBP/RESBP)

**SBP must be used with zzzPAT v 4.3 and above and WatchPAT™200/U
RESBP must be used with zzzPAT v 4.6 and above and WatchPAT™200U with
embedded 3.3228 and above**

Thank you for purchasing an Integrated Snore & Body Position Sensor.

Description

The integrated sensor consists internally of two sensors: a snore sensor and a body position sensor.

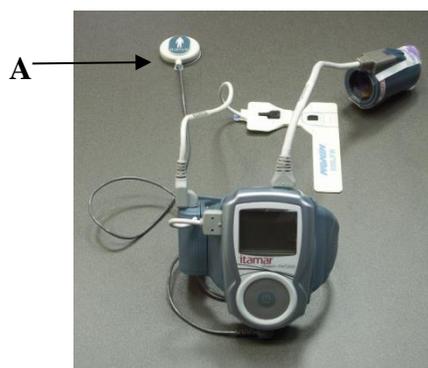


A - Integrated SBP sensor



A – SBP Sensor attachment
B - Sternal notch



A - Integrated RESBP sensor

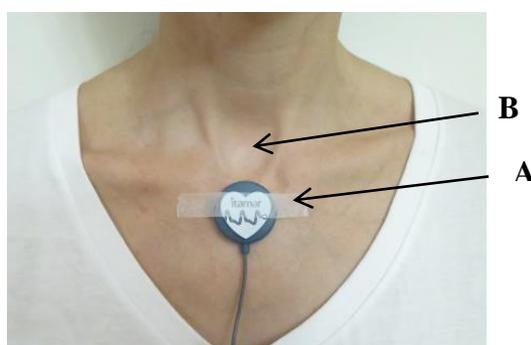

A-RESBP Sensor Attachment
B-Sternal notch

The integrated sensor is powered by the WatchPAT™ device and does not require a battery. It is automatically activated by the WatchPAT™ when plugged into the Snore & Body position port.

The **snore sensor** is an acoustic decibel detector. It uses a very sensitive microphone that responds to snoring and other sounds in the audio range and converts them to a small analog voltage that provides a clear, reliable indication of the presence of these sounds.

The **body position** sensor uses a 3-axis accelerometer that provides a signal directly proportional to the patient's sleeping posture (supine, prone, right, left and sit).

For RESBP only: The **chest movement signal** uses the same 3-axis accelerometer to provide raw chest movement signal data for measuring subject's breathing during the night.

Indications of use

The integrated Snoring & Body position sensor is an accessory of the WatchPAT™ home care device for use with patients suspected to have sleep related breathing disorders. The integrated sensor monitors the snoring level, which aids in the evaluation of the severity of sleep related breathing disorders, and the body position which aids in the evaluation of the type of sleep related breathing disorders. The RESBP sensor also provides raw chest movement signal data to measure the subjects breathing during the night.

Preparing the sensor

- Attach the round double sided adhesive sticker to the blue side of the sensor.

Applying the sensor

Make sure the room you are sleeping in is as quiet as possible during the night, turn off any possible noise sources. When using the SBP/RESBP it is advised to sleep alone in the room.

- The sensor is attached on the patient's chest right under the sternal notch. The sternal notch is the little U shape where the collar bones meet at the top of the breast bone.
- If needed, trim chest hair to ensure the sensor attached directly to your skin.
- To position the sensor attach it with the image standing up (cable pointing down), after peeling off the round adhesive sticker and pressing against the skin.
- Make sure the sensor is tight against the skin.
- Secure the sensor in place with medical tape.

Cleaning the sensor

Using 70% ethyl alcohol, thoroughly clean both sensor and cable.

SPECIFICATIONS	
Snoring Sensor Technology	Sensitive microphone
Body Position and Chest Movement (for RESBP only) Sensor Technology	3-axis Accelerometer
Signal Amplitude	0-3.3 V
Connector Type	1 mm medical safety connector plug from Plastics1 <i>Wire Length:</i> 3.2 foot (100 cm)
Physical Size	1.3 inch diameter (32 mm diameter)
Weight	12 gr
Warranty	6 months
Temperature	<i>Operation</i> 0 to 40 °C

Humidity	<i>Storage</i>	-20 to 40 °C
	<i>Transport</i>	-20 to 60 °C
Atmospheric pressure	<i>Operating, Storage & Transport</i>	0% – 93% (non-condensing)
	<i>Operating, & Storage Transport</i>	10 – 15 psi 8 – 15 psi

Snoring and Body Position Accuracy

This section gives statistical performance measure for Itamar SBP sensor, when used with the WatchPAT™ device.

I. Body Position

The body position measured by the WatchPAT™ device with Itamar SBP sensor was compared to the gold standard, manual scoring of the video recording of 31 patients, in 1 minute's epochs (total of 7111 epochs) during sleep.

The Agreement between the device and the video recording was 90%.


Simple Kappa agreement value was 0.8185 (95% confidence level of 0.8059 and 0.8311).

II. Snoring

The snoring level measured by the WatchPAT™ device with Itamar SBP sensor was compared to a gold standard PSG dB-meter placed 1 meter from patient's head. The study included 26 patients, and the analysis was done in 30sec epochs.

The correlation coefficient was calculated using Pearson method, assuming a linear relation between the results of the two devices. A statistically significant correlation was calculated between the two devices: $r=0.65$ p value <0.0001 .

The next figure shows a scatter plot of sleep disturbance Index produced by WatchPAT™ device and dB-meter, with linear regression line.

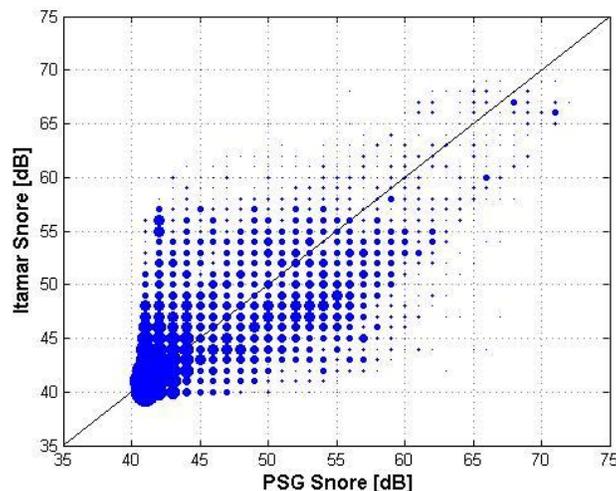


An estimation of the error in each snoring level was calculated by looking at the WatchPAT™ device measurement cut by the results of dB-meter in intervals of 1 dB in the range of above 40dB (below 40 dB was considered not clinically significant being background noise). A high correlation was observed between the results of the two devices for the range of 40-70dB (where sufficient data points were gathered), meaning the resemblance in the results uniformly existed for all the snore levels measured.


The next table presents the statistics of WatchPAT™ device measurements per dB-meter calculation at that range.

PSG DB Value	N	Mean	Std	Coef. Of Variation [%]	Min	Max	Median	Lower 95% CI	Upper 95% CI
40	2033	41.10	1.89	4.60	40	54	40	41.01	41.18
41	1319	41.61	2.67	6.43	40	54	41	41.47	41.76
42	908	42.68	3.79	8.88	40	62	41	42.44	42.93
43	746	44.12	4.49	10.19	40	58	42	43.80	44.44
44	719	44.75	4.65	10.39	40	65	43	44.41	45.09
45	643	45.90	5.07	11.04	40	59	45	45.51	46.30
46	602	46.45	5.17	11.13	40	59	46	46.04	46.86
47	590	47.39	5.31	11.21	40	66	47	46.96	47.82
48	568	48.03	5.17	10.76	40	61	49	47.60	48.45
49	414	48.56	5.33	10.97	40	64	49	48.05	49.08
50	369	49.07	5.27	10.75	40	61	49	48.53	49.60
51	334	49.68	5.66	11.39	40	63	50	49.07	50.28
52	335	50.00	5.58	11.17	40	64	51	49.39	50.59
53	311	51.18	5.56	10.86	40	63	51	50.56	51.79
54	253	51.71	5.78	11.19	40	66	52	51.00	52.42
55	209	51.85	5.49	10.59	40	66	52	51.11	52.60
56	182	51.91	5.62	10.82	40	64	52	51.09	52.72
57	129	52.29	5.91	11.30	41	64	52	51.26	53.32
58	95	54.94	5.94	10.82	42	67	55	53.73	56.15
59	66	55.53	6.37	11.47	42	66	55.5	53.97	57.10
60	72	57.82	5.92	10.24	44	66	58	56.43	59.21
61	58	58.48	6.31	10.78	43	68	58.5	56.82	60.14
62	43	59.47	6.56	11.02	46	68	60	57.45	61.48
63	32	59.63	4.15	6.96	50	67	59	58.13	61.12
64	15	62.53	3.93	6.28	56	68	64	60.36	64.71
65	22	64.41	6.21	9.64	49	70	67	61.66	67.16
66	48	66.90	3.66	5.48	59	70	68.5	65.83	67.96
67	42	65.76	3.28	4.99	60	71	67	64.74	66.78
68	27	64.56	2.67	4.13	55	68	65	63.50	65.61
69	6	67	2.37	3.53	64	70	67	64.52	69.48

The results are also presented in the next figure. The figure presents the mean WatchPAT™ device with SD error bar.

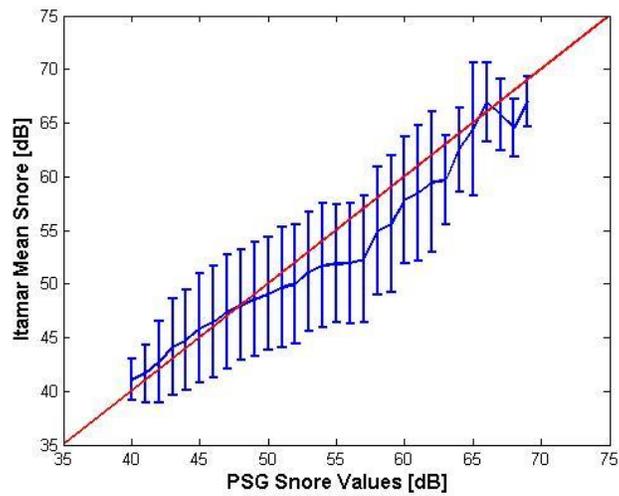

Summary statistics (mean \pm SD) of WatchPAT™200U device by dB-meter levels



Note

The snoring and body position safety and effectiveness was validated on adult population only.

APPENDIX B: Tamper-proof testing with WatchPAT™

	WatchPAT™ 200U	Action	Comment
Important Note	Important Note	This short guide will instruct a WatchPAT trained operator on how to perform Tamper-Proof testing with the WatchPAT. For complete WatchPAT training and instructions please refer to the WatchPAT user manual and to the zzzPAT user manual.	<ul style="list-style-type: none"> • Make sure the zzzPAT version is: 4.4.64 or higher • Make sure the WatchPAT embedded software version is: 3.2217 or higher • Make sure you enable the "Tamper-Proof Testing" option from the zzzPAT "Setup" menu > "General Settings"
Study Preparation	1 New Study on zzzPAT	While preparing the new study on the zzzPAT (refer to the user manual for detailed instructions), check the box "Study with Tamper-Proof Testing" at the bottom of the "New Study" screen. Note: Once you enable this option you MUST use a bracelet for the night study. The WatchPAT will NOT function without a bracelet connected to it.	
Bracelet Preparation	2 Bracelet	Select a Tamper-Proof Bracelet for the study.	
Bracelet Preparation	3 Connecting the Cable to the WatchPAT	Connect the gray cable with the red and white snap buttons to the WatchPAT socket.	
Bracelet Preparation	4 Connecting the Bracelet	Connect the red and white snap buttons to the red and white snaps on the bracelet respectively.	

	WatchPAT™ 200U	Action	Comment
Bracelet Preparation	<p>5 Pairing WatchPAT with Bracelet: Site-Diagnostic Test</p>	<p>Make sure the bracelet is connected before starting the test. Perform the standard site diagnostic test ("device test" as described in the user manual).</p> <p>After test is completed, disconnect the bracelet from the WatchPAT and store it in the WatchPAT case.</p> <p>Note: Once the "device test" is successfully done with the bracelet connected - the specific bracelet must be used for the following night recording.</p>	
Patient Preparation	<p>6 Placing Bracelet on Patient</p>	<ul style="list-style-type: none"> Make sure you have all 3 parts: bracelet and two white plastic clips. Place the bracelet upside down on a flat surface (white side facing up). <ol style="list-style-type: none"> Insert the white plastic clip into the two separated holes (flat side facing up). Wrap the bracelet around the wrist of the non-dominant arm (tested arm) of the patient. Insert the white plastic clips into the holes. Make sure it is snug but not too tight. If there is some loose strap left, fold it and re-insert it into the holes. <p>DO NOT CUT LOOSE STRAP - CUTTING IT WILL RENDER THE BRACELET UNUSABLE</p> <ol style="list-style-type: none"> Secure the bracelet by placing the second white plastic clip on-top of the first. Make sure it is secured tightly. 	    
Patient Guidance	<p>7 Explain to Patient</p>	<ul style="list-style-type: none"> The patient may choose to perform the study during any night of the week. The patient may shower with the bracelet. Instruct patient to connect the red and white snap buttons to the red and white snaps on the bracelet respectively. Instruct patient to turn on the WatchPAT only after it is connected to the bracelet. THE BRACELET SHOULD NOT BE REMOVED UNTIL THE NIGHT STUDY IS COMPLETED. Removing the bracelet before or during the night will cause the device to shut down. In the morning, instruct the patient to cut the bracelet along the dotted line by using small scissors and to put it in the WatchPAT case along with all the other parts (DO NOT THROW THE BRACELET AWAY). <p>Do not try to connect ANY other device to the bracelet.</p>	

APPENDIX C: LICENSE AGREEMENT

License To Operator From Itamar

IMPORTANT – PLEASE READ THIS LICENSE AGREEMENT CAREFULLY BEFORE INSTALLING OR OTHERWISE USING THE LICENSED SOFTWARE (AS DEFINED BELOW) OR THE PRODUCT WITH WHICH YOU RECEIVED THIS LICENSE AGREEMENT. THIS LICENSE AGREEMENT APPLIES TO (a) ALL LICENSED SOFTWARE, (b) ALL LICENSED PRODUCTS (AS DEFINED BELOW), AND (c) ALL THIRD PARTY PRODUCTS INTO WHICH A LICENSED PRODUCT OR LICENSED SOFTWARE IS INCORPORATED. SHOULD YOU HAVE ANY QUESTIONS CONCERNING THIS LICENSE AGREEMENT, PLEASE CONTACT THE VENDOR FROM WHICH YOU PURCHASED THE LICENSED SOFTWARE, LICENSED PRODUCT, OR PRODUCT INTO WHICH A LICENSED PRODUCT OR LICENSED SOFTWARE IS INCORPORATED. YOU MAY ALSO CONTACT ITAMAR AT THE ADDRESS PROVIDED AT THE END OF THIS LICENSE AGREEMENT.

This License Agreement is a legal agreement between you (as an individual, company, organization or other entity) and Itamar Medical Ltd. (“Itamar”). By installing, copying, or otherwise using the Licensed Software, and/or by using the Licensed Product or third party product into which a Licensed Product or Licensed Software is incorporated (“Third Party Product”), you agree to be bound by the terms of this License Agreement with respect to the Licensed Software and Licensed Products. If you do not agree to the terms of this License Agreement, including, without limitation, the Restrictions on Use as provided in Section 2 do not install, use or copy the Licensed Software or use the Licensed Product or the Third Party Product.

The Licensed Software and the Licensed Products are protected by US patent laws, trade secret laws, copyright laws, and international treaty provisions as well as other intellectual property laws and treaties. Therefore, you must treat the Licensed Software and the Licensed Products like any other copyrighted and protected material or product. All title to the Licensed Software and all intellectual property rights in and to the Licensed Software and the Licensed Products shall remain with Itamar.

1. DEFINITIONS

- 1.1. “Licensed Product(s)” means *the Watch_PAT200 (Watch-PAT200), the Site_PAT200, the uPAT Probe* and the corresponding components of any Third Party Product with which this License Agreement was received. Some Licensed Products are stand-alone products and some Licensed Products are incorporated as components within Third Party Products, in each case sold or otherwise made available, by Itamar and/or third parties. If you have received this License Agreement with a Third Party Product, this License Agreement applies only to the Licensed Product**

incorporated as a component within such Third Party Product.

1.2. “Licensed Software” means the *zzzPAT* software, the associated media and accompanying materials provided to you with such *zzzPAT* software. Some Licensed Software is a stand-alone product and some Licensed Software is incorporated as a component within a Licensed Product, in each case sold or otherwise made available, by Itamar and/or third parties. If you have received this License Agreement with a Licensed Product which incorporates the Licensed Software as a component within such Licensed Product, this License Agreement applies to the Licensed Software.

2. GRANT OF LICENSE AND RESTRICTIONS ON USE

2.1 Itamar hereby grants you a non-exclusive right to use the Licensed Software , solely for its intended use in sleep medicine (with the term "sleep medicine" including Cheyne-Stokes respiration as well as research in sleep medicine and Cheyne-Stokes respiration) (i) with the Licensed Product(s) and (ii) in accordance with the provisions of this License Agreement and the instructions provided in the documentation accompanying the Licensed Software and the Licensed Product You may make one copy of the Licensed Software solely for backup or archival purposes, or transfer the Licensed Software to a single hard disk, provided you keep the original solely for backup or archival purposes. However, you may not cause any Licensed Software which is not designed for use on a server, to execute or be loaded into the active memory or media of more than one computer at any one time.

2.2 Any use of the Licensed Software and/or Licensed Product other than as set forth in Section 2.1 above is strictly forbidden. Without derogating from the generality of the above, you may not:

- distribute, reproduce, copy, assign, rent, lease, or otherwise transfer the rights granted to you under this License Agreement to any third party except explicitly as set forth in this License Agreement;
- reverse engineer, decompile, or disassemble, as applicable, the Licensed Software or the Licensed Product, except as expressly permitted by applicable law; or
- modify in any manner the Licensed Software and/or the Licensed Product unless obtaining the prior written consent of Itamar.

3. TRADEMARKS

Cardio-PAT™, Sleep-PAT™ and all trademarks and logos, which appear on or in connection with the Licensed Software and/or the Licensed Products, as may be amended from time to time, are, unless stated otherwise, trademarks of Itamar. No right, license, or interest to such trademarks are generated or granted hereunder other than the limited right to use provided herein, and you agree that no such right, license, or interest shall be asserted by you with respect to such trademarks. You may not remove or destroy any

copyright, trademark, logo or other proprietary marking or legend placed on or contained in the Licensed Software or a Licensed Product.

4. LIMITED WARRANTIES AND DISCLAIMERS

a. Against Infringement. Itamar hereby warrants to you that it has the right to grant you the license to use the Licensed Software and/or the Licensed Product and to enter into this License Agreement and that neither the Licensed Software nor the Licensed Product(s) infringes the intellectual property rights of any third party.

b. As to Licensed Product. Itamar warrants that the Licensed Product with which this License Agreement was delivered, will be free from defects in design, materials and workmanship for a period of one year from the date of delivery of the Licensed Product to you. If the Licensed Product contains a defect in design, materials or workmanship and such Licensed Product is returned to Itamar within one (1) year of delivery of the Licensed Product to you, Itamar will repair or replace the Licensed Product, or issue a credit for the purchase price of the Licensed Product, with the choice to repair, replace or credit being within the sole discretion of Itamar. The foregoing repair, replacement or credit remedy will be your sole remedy for breach of the warranty set forth in this Section 4(b).

c. As to Licensed Software. Itamar warrants that for a period of ninety (90) days from the date of delivery of the Licensed Software to you, the Licensed Software will, under normal use, be free from defects in materials and workmanship and will perform substantially as it is intended to perform. If during such ninety (90) day period, the Licensed Software has a defect in materials or workmanship or does not perform substantially as it is intended to perform, Itamar shall (a) attempt to correct or assist you around errors with efforts which Itamar believes suitable to the problem, (b) replace the Licensed Software with a functionally equivalent software, or (c) issue a credit for the purchase price of the Licensed Software, with the choice to correct or assist, replace or credit being within the sole discretion of Itamar. The foregoing correct or assist, replacement or credit remedy will be your sole remedy for breach of the warranty set forth in this Section 4(c).

d. Limitation of Warranties. The warranties contained in Sections 4(b) and 4(c) above do not cover damage to the Licensed Products or the Licensed Software caused by accident, misuse, abuse, negligence, failure to install in accordance with Itamar's installation instructions, failure to operate under conditions of normal use and in accordance with the terms of the documentation accompanying the Licensed Product and/or the Licensed Software, failure to maintain in accordance with applicable documentation accompanying the Licensed Product and/or the Licensed Software, alteration or any defects not related to materials or workmanship, or in the case of Licensed Products, design, materials or workmanship. This warranty does not cover damage which may occur in shipment. This warranty does not apply to Licensed Products and/or Licensed Software not purchased new. This warranty does not apply to any Licensed Product or any individual parts of a Licensed Product which have been repaired or altered by anyone other than Itamar or a person or entity authorized by Itamar to repair Licensed Products.

While every reasonable effort has been made to ensure that you will receive Licensed Software that you can use, Itamar does not warrant that the functions of the Licensed Software will meet your requirements or that the operation of the Licensed Software will be uninterrupted or error free. Itamar is not responsible for problems caused by changes in the operating characteristics of the hardware or operating system software you are using, nor for any problems in the interaction of the Licensed Software with non-Itamar software.

ITAMAR HEREBY DISCLAIMS, WITH RESPECT TO THE LICENSED PRODUCTS AND THE LICENSED SOFTWARE, ALL OTHER WARRANTIES AND CONDITIONS, WHETHER EXPRESS OR IMPLIED, INCLUDING, BUT NOT LIMITED TO, ANY WARRANTIES OR CONDITIONS OF OR RELATED TO MERCHANTABILITY, FITNESS FOR A PARTICULAR PURPOSE, ACCURACY OR COMPLETENESS OF INFORMATION, LACK OF NEGLIGENCE AND CORRESPONDENCE TO DESCRIPTION.

5. LIMITATION OF LIABILITY

(A) TO THE MAXIMUM EXTENT PERMITTED BY APPLICABLE LAW, EXCEPT FOR DAMAGES ARISING UNDER SECTION 4(A) ABOVE, IN NO EVENT SHALL ITAMAR BE LIABLE TO YOU FOR DAMAGES IN EXCESS OF THE PURCHASE PRICE YOU PAID FOR THE LICENSED SOFTWARE, THE LICENSED PRODUCT OR THE APPLICABLE THIRD PARTY PRODUCT. THE FOREGOING LIMITATION SHALL BE APPLICABLE REGARDLESS OF WHETHER THE ACTION GIVING RISE TO SUCH DAMAGES IS IN TORT, CONTRACT, STRICT PRODUCTS LIABILITY, OR OTHERWISE.

(B) IN NO EVENT SHALL ITAMAR BE LIABLE FOR ANY SPECIAL, INCIDENTAL, INDIRECT OR CONSEQUENTIAL DAMAGES WHATSOEVER ARISING OUT OF OR IN ANY WAY RELATED TO THE USE OF OR INABILITY TO USE THE LICENSED SOFTWARE AND/OR THE LICENSED PRODUCT AND/OR THE THIRD PARTY PRODUCT, OR THE PROVISION OF OR FAILURE TO PROVIDE SUPPORT SERVICES BY ITAMAR, EVEN IF ITAMAR HAS BEEN ADVISED OF THE POSSIBILITY OF SUCH CONSEQUENTIAL DAMAGES. THE FOREGOING DISCLAIMER OF CONSEQUENTIAL DAMAGES SHALL BE APPLICABLE REGARDLESS OF WHETHER THE ACTION GIVING RISE TO SUCH DAMAGES IS IN TORT, CONTRACT, STRICT PRODUCTS LIABILITY, OR OTHERWISE.

(C) IN ORDER TO BE ENTITLED TO INDEMNIFICATION HEREUNDER IN CONNECTION WITH AN INFRINGEMENT CLAIM, YOU MUST (i) NOTIFY ITAMAR IN WRITING PROMPTLY UPON BECOMING AWARE OF AN INFRINGEMENT CLAIM OR THE POSSIBILITY THEREOF, (ii) GRANT ITAMAR SOLE CONTROL OF THE SETTLEMENT, COMPROMISE, NEGOTIATION AND DEFENSE OF ANY SUCH ACTION, AND (iii) PROVIDE ITAMAR WITH ALL INFORMATION RELATED TO THE ACTION THAT IS REASONABLY REQUESTED BY ITAMAR. NOTWITHSTANDING THE FOREGOING, ITAMAR SHALL HAVE

NO INDEMNIFICATION OBLIGATIONS WITH RESPECT TO ANY INFRINGEMENT CLAIM TO THE EXTENT ARISING FROM YOUR USE OF THE LICENSED PRODUCT AND/OR LICENSED SOFTWARE IN CONJUNCTION WITH OTHER HARDWARE OR SOFTWARE WHERE USE WITH SUCH OTHER HARDWARE OR SOFTWARE GAVE RISE TO THE INFRINGEMENT CLAIM.

6. TERMINATION

Without prejudice to any other rights or remedies, Itamar may terminate this License Agreement immediately if you fail to comply with any of its terms and conditions. In the event of such termination, you must, within ten (10) business days of receiving notice of termination from Itamar, cease all use of the Licensed Software and destroy all copies thereof, and cease all use of the Licensed Product (including Licensed Product incorporated within Third Party Product).

7. TRANSFERABILITY

You may only transfer or assign the rights and obligations hereunder together with the Licensed Software and/or the Licensed Product or Third Party Product as a whole, without retaining any rights or, subject to Sections 2 and 3 above, any obligations arising after the date of such transfer or assignment, or retaining any installed or uninstalled copy of the Licensed Software, the Licensed Product or the Third Party Product. Any attempt by you to rent, lease, sublicense, assign or transfer any of the rights, duties or obligations hereunder in any other way is forbidden and shall be null and void.

8. SEVERABILITY

Should any term or provision of this License Agreement be declared void or unenforceable by any court of competent jurisdiction in any country or countries, such declaration shall have no effect on the remainder of this License Agreement in such country or countries, or on this License Agreement in other countries.

9. NO WAIVER

The failure of either party to enforce any rights granted to it hereunder or to take action against the other party in the event of any breach hereunder shall not be deemed a waiver by that party as to subsequent enforcement actions in the event of future breaches.

10. GOVERNING LAW AND JURISDICTION

This License Agreement is governed by the laws of the State of New York, excluding its conflict of laws principles. The United Nations Convention on Contracts for the International Sale of Goods shall not apply to any of the transactions contemplated by this License Agreement.

11. ENTIRE UNDERSTANDING

This License Agreement represents the complete and exclusive understanding between you and Itamar concerning the license by Itamar to you of Licensed Software and Licensed Products and supersedes all prior agreements and representations between the parties with respect to the subject matter hereof, unless specifically stated otherwise in a writing signed by Itamar and you. This License Agreement may not be amended other than by a written agreement specifically intended for this purpose and signed by Itamar and you.

Note: Should you have any questions concerning this License Agreement, or if you desire to contact Itamar for any reason, please write to:

USA:

Itamar Medical Inc.
3290 Cumberland Club Drive, Suite 100
Atlanta, Georgia 30339, USA
Tel: 1 888 748 2627

Worldwide:

Itamar Medical Ltd.
9 Halamish St., P.O.Box 3579
Caesarea Ind. Park, 3088900, Israel
Tel: +972 4 617 7000

APPENDIX D: REGULATORY REPRESENTATIVE

Itamar Medical's authorized regulatory representative is:



Arazy Group GmbH

The Squire 12, Am Flughafen,
60549 Frankfurt am Main,
Germany

APPENDIX E: DESCRIPTION OF THE WATCHPAT™200U UPAT PROBE

The WatchPAT uPAT probe is an opto-pneumatic finger-mounted probe.

Its role is to continuously measure the relative state of the vasomotor activity in the distal part of the finger based on a plethysmographic method. The uPAT probe is designed to cover the distal part of the finger with a uniform pressure field extending to the tip of the finger. This design prevents venous blood pooling, engorgement and stasis, which inhibits retrograde venous shock wave propagation, and allows partial unloading of arterial wall tension that significantly improves the dynamic range of the measured signal. The optic component of the probe measures the optical density related changes of the arterial blood volume in the digital arteries, associated with each heartbeat. Peripheral arterial constrictions, when present, are shown by attenuation in the PAT signal amplitude, a marker of sympathetic activation.

The uPAT probe also measures the changes in absorbance of the finger at both red and infrared light at peak wavelengths of 660nm and 910nm respectively. The maximum optical output power is 65mW. These measurements are used to calculate the oximetry signal in an offline program according to the pulse oximetry principles.

The uPAT probe is an integral part of the WatchPAT™ device and is to be used only with the WP200U device.

APPENDIX F: MANUFACTURING DECLARATIONS ACCORDING TO IEC 60601-1 & 60601-1-2

Notes

- The Itamar Medical's WatchPAT™200U (WP200U) requires special precautions with regard to electromagnetic compatibility.
- It must be installed and prepared for use as described in section 3 - Preparation for Sleep Study.
- Certain types of mobile telecommunication devices such as mobile telephones are likely to interfere with the Itamar Medical's WP200U.
- The recommended separation distances in this paragraph must therefore be complied with.
- The Itamar Medical's WP200U must not be used near or on top of another device. If this cannot be avoided, it is necessary – before clinical use – to check the equipment for correct operation under the conditions of use.
- The use of accessories other than those specified or sold by Itamar Medical as replacement parts may have the consequence of increasing the emissions or decreasing the immunity of the unit.
- To ensure “Isolation means” disconnect the power supply.

Electromagnetic Compatibility

Electromagnetic Emissions

- Itamar Medical's WP200U is intended for use in the electromagnetic environment specified in the following tables 1, 2, 4, 6 and 9 below.
- The user and/or installer of the unit must ensure that it is used in such an environment.

Table 1 – based on IEC 60601-1-2:2014		
Guidance and manufacturer's declaration – electromagnetic emissions – WP200U		
The WP200U is intended for use in the electromagnetic environment specified below; The customer or the user of the WP200U should assure that it is used in such an environment.		
Emissions test	Compliance	Electromagnetic environment - guidance
RF emissions CISPR 11	Group 1	The WP200U uses RF energy only for its internal function. Therefore, its RF emissions are very low and are not likely to cause any interference in nearby electronic equipment. Conducted emission: Frequency: 1MHz-30MHz Peak current limit: 24 (dBuA) Radiated emission: Frequency: 30MHz-1GHz
RF emissions CISPR 11	Class B	The WP200U is suitable for use in all establishments, including domestic establishments and those directly connected to the public low-voltage power supply network that supplies buildings used for domestic purposes.
Harmonic emissions IEC 61000-3-2	Class A	

Table 2 - based on IEC 60601-1-2:2014

Guidance and manufacturer's declaration – electromagnetic immunity – WP200U			
The WP200U is intended for use in the electromagnetic environment specified below; The customer or the user of the WP200U should assure that it is used in such an environment.			
Immunity test	IEC 60601-1-2 Test level	Compliance level	Electromagnetic environment - guidance
Electrostatic discharge (ESD) IEC 61000-4-2	±8 kV contact ±15 kV air	±8 kV contact ±15 kV air	Floors should be wood, concrete or Ceramic tile. If floors are covered with synthetic material, the relative humidity Should be at least 30 %.
Power frequency (50/60 Hz) magnetic field IEC 61000-4-8	30 A/m	30 A/m	Power frequency magnetic fields should be at levels characteristic of a typical public low-voltage power supply network that supplies buildings used for domestic purposes, commercial or hospital, clinic environment.
NOTE: UT is the a.c. mains voltage prior to application of the test level.			

Table 4 - based on IEC 60601-1-2:2014

Guidance and manufacturer's declaration – electromagnetic immunity – WP200U			
The WP200U is intended for use in the electromagnetic environment specified below; The customer or the user of the WP200U should assure that it is used in such an environment.			
Immunity test	IEC 60601-1-2 Test level	Compliance level	Electromagnetic environment - guidance
Conducted RF IEC 61000-4-6	3 Vrms outside ISM band 6 Vrms in the ISM band 150 k Hz to 80 MHz	3 Vrms 6 Vrms	Portable and mobile RF communications equipment should be used no closer to any part of the WP200U , including cables, than the recommended separation distance calculated from the equation applicable to the frequency of the transmitter. Recommended separation distance $d = 1.17\sqrt{P}$ $d = 0.58\sqrt{P}$
Radiated RF IEC 61000-4-3	10 V/m 80 MHz to 2,5 GHz <u>Home Healthcare</u> 80MHz-2.7GHz (10V/m) <u>Professional healthcare</u> 80MHz-2.7GHz (3V/m) 80% AM 1KHz	10 V/m	$d = 0.35\sqrt{P}$ 80 M Hz t o 800 MHz $d = 0.7\sqrt{P}$ 800 MHz t o 2,7 GHz where P is the maximum output power rating of the transmitter in watts (W) according to the transmitter manufacturer and d is the recommended separation Distance in meters (m). Field strengths from fixed RF transmitters, as

			<p>determined by an electromagnetic site survey ,^a should be less than the compliance level in each frequency range .^d</p> <p>Interference may occur in the vicinity of equipment marked with the following symbol:</p> 
<p>NOTE 1 At 80 MHz and 800 MHz, the higher frequency range applies.</p>			
<p>NOTE 2 These guidelines may not apply in all situations .Electromagnetic propagation is affected by absorption And reflection from structures objects and people.</p>			
<p>a Field strengths from fixed transmitters, such as base stations for radio (cellular/cordless) telephones and land mobile radios, amateur radio, AM and FM radio broadcast and TV broadcast cannot be predicted theoretically with accuracy. To assess the electromagnetic environment due to fixed RF transmitters, an electromagnetic site survey should be considered. If the measured field strength in the location in which the WP200U is used exceeds the applicable RF compliance level above, the WP200U should be observed to verify normal operation. If abnormal performance is observed, additional measures may be necessary, such as re-orienting or relocating the WP200U.</p> <p>b Over the frequency range 150 kHz to 80 MHz, field strengths should be less than 3 V/m.</p>			

Recommended Separation Distances

The Itamar Medical's WP200U is intended for use in an electromagnetic environment in which radiated radiofrequency disturbances are controlled.

The user and/or installer of the unit can help prevent electromagnetic interference by maintaining a minimum distance between portable and mobile radiofrequency communications equipment (emitters) and the Itamar Medical's WP200U, according to the maximum output power of the equipment, as recommended in the table below.

Table 6 - based on IEC 60601-1-2:2014				
Recommended separation distances between portable and mobile RF communications equipment and the WP200U				
Rated maximum output power of transmitter	Separation distance according to frequency of transmitter (in meters)			
	Meters [m]			
	150kHz to 80MHz	150kHz to 800MHz	80MHz to 800MHz	800MHz to 2.5GHz
Watts [W]	$d = 1.17\sqrt{P}$ (3Vrms)	$d = 0.58\sqrt{P}$ (6Vrms)	$d = 0.35\sqrt{P}$	$d = 0.7\sqrt{P}$
0.01	0.12	0.06	0.04	0.07
0.1	0.37	0.18	0.11	0.22
1	1.17	0.58	0.35	0.7
10	3.7	1.83	1.11	2.21
100	11.7	5.8	3.5	7

For transmitters rated at a maximum output power not listed above, the recommended separation distance d in meters (m) can be estimated using the equation applicable to the frequency of the transmitter, where P is the maximum output power rating of the transmitter in watts (W) according to the transmitter manufacturer.

NOTE 1 At 80 MHz and 800 MHz, the separation distance for the higher frequency range applies.
NOTE 2 These guidelines may not apply in all situations. Electromagnetic propagation is affected by absorption and reflection from structures, objects, and people.

Table 9 - based on IEC 60601-1-2:2014							
Proximity Fields from RF Wireless Communication Equipment							
Test frequency (MHz)	Band ^{a)} (MHz)	Service ^{a)}	Modulation ^{b)}	Maximum power (W)	Distance (m)	Immunity TEST LEVEL (V/m)	Minimum separation distance [m]
385	360-390	TETRA 400	Pulse modulation ^{b)} 18 Hz	1.8	0.3	27	0.3
450	430-470	GMRS 460, FRS 460	FM ^{c)} ±5 kHz deviation 1 kHz sine	2	0.3	28	0.3

710	704-787	LTE Band 13,17	Pulse modulation ^{b)} 217 Hz	0.2	0.3	9	0.3
745							
780							
810	800-960	GSM 800/900. TETRA 800. CDMA 850. LTE Band 5	Pulse modulation ^{b)} 217 Hz	2	0.3	28	0.3
870							
930							
1720	1 700- 1 990	GSM 1800; CDMA 1900; DECT; LTE Band 1, 3, 4, 25; UMTS	Pulse modulation ^{b)} 217 Hz	2	0.3	28	0.3
1845							
1970							
2450	2 400- 2 570	Bluetooth, WLAM, 802.11 b/g/n, RFID 2450, LTE Band 7	Pulse modulation ^{b)} 217 Hz	2	0.3	28	0.3
5240	5 100- 5 800	WLAM 802.11 a/n	Pulse modulation ^{b)} 217 Hz	0.2	0.3	9	0.3
5500							
5785							
NOTE if necessary to achieve the IMMUNITY test level, the distance between the transiting antenna and the ME equipment or ME system may be reduced to 1m. The 1m test distance is permitted by IEC 61000-4-3.							
<p>a) For some services, only the uplink frequencies are included</p> <p>b) The carrier shall be modulated using a 50% duty cycle square wave signal.</p> <p>c) As an alternative to FM modulation, 50% pulse modulation at 18Hz may be used because while it does not represent actual modulation, it would be worst case.</p>							

The MANUFACTURER should consider reducing the minimum separation distance, based on RISK MANAGEMENT, and using higher IMMUNITY TEST LEVELS that are appropriate for the reduced minimum separation distance. Minimum separation distances for higher IMMUNITY TEST LEVELS shall be calculated using the following equation:

$$E = \frac{6}{d} \sqrt{P}$$

Where P is the maximum power in W, d is the minimum separation distance in m, and E is the IMMUNITY TEST LEVEL in V/m.


APPENDIX G: SPO2 ACCURACY IN THE WATCHPAT™200U

The WatchPAT™200U device uses Itamar Medical Pulse Oximetry system for the measurement of functional oxygen saturation of arterial haemoglobin (SpO2). This appendix includes information regarding the accuracy of these measurements following a clinical study of Itamar Medical Pulse Oximetry.

1. Overall, the Arms is estimated to be 2.1 for the range 70-100%
2. The next table shows SpO2 Accuracy Results:

Test Device	SpO2 67-100% A_{RMS} / Bias	SpO2 90-100% A_{RMS} / Bias	SpO2 80-90% A_{RMS} / Bias	SpO2 70-80% A_{RMS} / Bias
WatchPAT™200U Finger Sensor Set 2 – H series	A _{RMS} 2.1 (726 pts) Bias 0.6	A _{RMS} 1.4 (255 pts) Bias -0.6	A _{RMS} 1.9 (227 pts) Bias 0.9	A _{RMS} 2.7 (225 pts) Bias 1.5


3. The next table shows the Bland-Altman plot for Itamar-Medical WP200U:

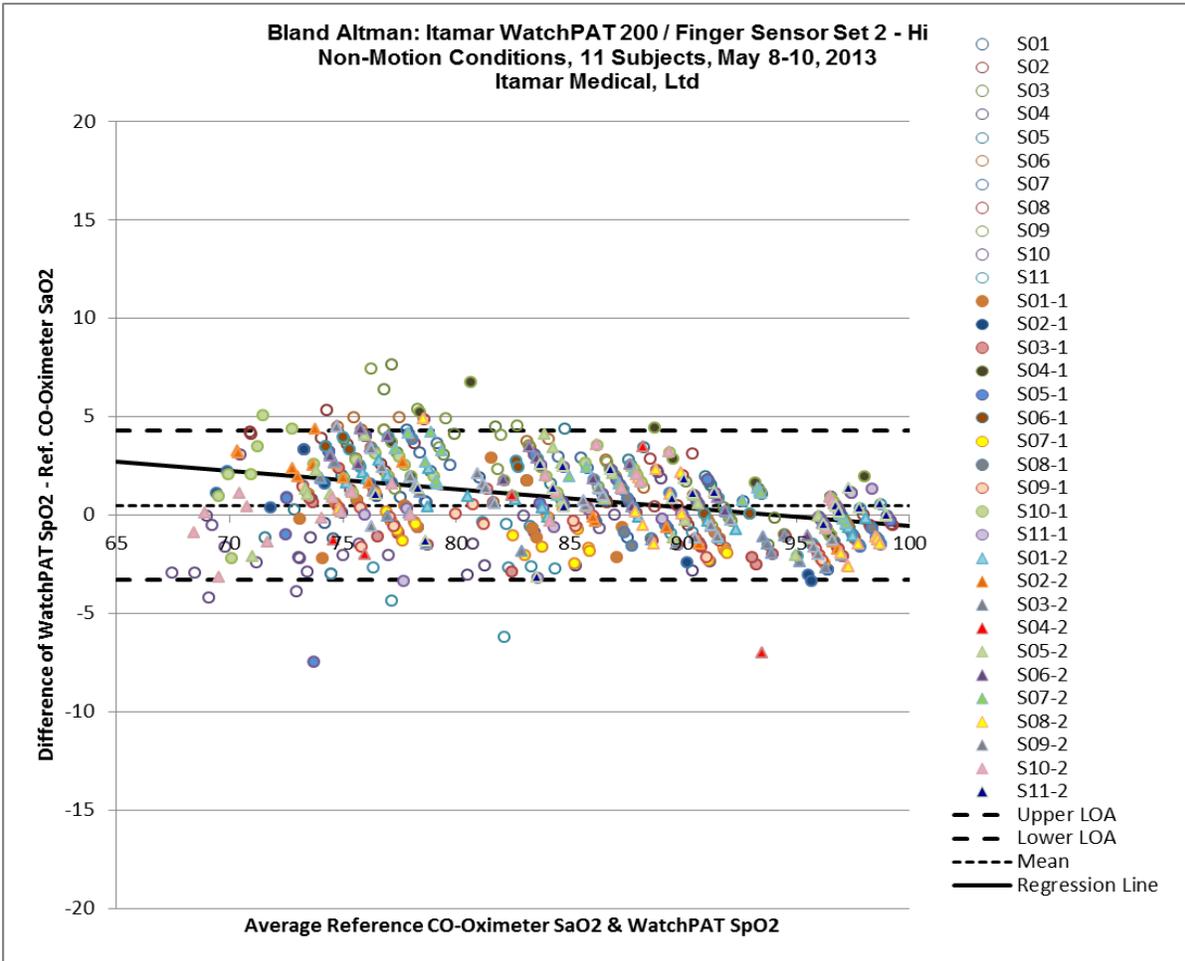

Reference: CO-Oximetry Range	68-99%
Linear Regression (Bland Altman)	$y = -0.0931x + 8.7875$
Mean Bias	0.51
# pts	726
Upper 95% Limits of Agreement	4.3
Lower 95% Limits of Agreement	-3.3

*Source of data:

Title:	Itamar SpO2 Accuracy Validation vs Reference CO-Oximetry, PR2013-062
Date:	2013-08-20
Clinical Investigator(s):	Clinimark 80 Health Park Drive, Suite 20 Louisville, Colorado 80027, USA
Sponsor:	Itamar Medical, Ltd. 9 Halamish St POB 3579, Caesarea 3088900 Israel
Device(s):	Non-Motion: Itamar Medical WatchPAT 200 Pulse Oximetry
Study Date(s):	May 8-10, 2013



Note

A Functional tester cannot be used to assess the accuracy of the internal pulse oximeter.

APPENDIX H: WP200U EFFECTIVENESS IN DETECTING CENTRAL SLEEP APNEA SYNDROME USING A THRESHOLD OF AHIC=10

The efficacy of the WP200U in the detection of AHIC for a threshold of 10 was evaluated in a multi-center study in 72 patients and the following results were obtained:

- Sensitivity = 70.6%
- Specificity = 87.3%
- Positive predictive value (PPV) = 63.2%
- Negative predictive value (NPV) = 90.6%

In addition the following statistics was demonstrated:

Area Under the Curve (AUC) = 0.873 of an ROC for a PSG threshold of AHIC = 10

Pearson correlation between AHIC of PSG and WP200U of R=0.83 with a slope of 0.91 and offset of 0.26

ADDITIONAL NON-DIAGNOSTIC INFORMATION

The efficacy of the WP200U in the assessment of %CSR (Cheyne Stokes Breathing) pattern was evaluated in a sub-group of 17 patients that were found to have AHIC \geq 10 by the PSG on a standard 30 seconds epoch-by-epoch comparison¹. A total of 10,509 aggregated epochs were derived from these patients and the following results were obtained:

- Sensitivity = 51.3%
- Specificity = 93.7%
- Positive Predictive Value (PPV) = 78.4%
- Negative Predictive Value (NPV) = 81.3%
- Overall Agreement = 80.7%

*Source of Data:

Study Title: Diagnosis of Sleep-related Respiratory Disorders in patients suspected of having SDB with and without cardiac disorders

Date of the Report: May 25, 2016

Principal Investigator(s): Prof. Giora Pillar (Carmel Medical Center)

Sponsor: Itamar Medical, Ltd. 9 Halamish St POB 3579, Caesarea 38900 Israel

Device(s): Watch PAT 200U (WP200U)

Study Period: September 5, 2015 to February 24 2016

National Clinical Trial (NCT) Numbers: NCT02369705, NCT01570738

¹ %CSR indication is not cleared by FDA.

APPENDIX I: ZZZPAT HARDWARE REQUIREMENTS

Hardware configuration:

Computer Pentium 4 3GHz or higher

1 available USB port

XGA screen resolution (minimum 1024 x 768 pixels) Colors set to 16 bits or higher

RAM 1GB or higher

Disk space requirements:

- **Standalone installation**

- 10GB minimum / 60GB recommended disk space on Files folder and at least 1.2GB on boot drive

- **Shared installation**

- SQL DB drive – 1.2GB if using our default MS SQL Express installation and enough for 1 year worth of studies (500 KB / study).
- Shared Files folder for raw data signal files - enough for 1 year worth of studies (30 MB / study).

Operating System:

Windows Server 2008 Service Pack 1 and above

Windows 7 with Service Pack 1 and above

APPENDIX J: SPARE PARTS LIST

The following items can be ordered and purchased individually:

- uPAT probe (a box of 12 uPAT probes)
- uPAT probe connection cable
- Wrist Strap
- Snore and Body Position sensor (SBP)
- Snore and Body Position sensor (RESBP)
- Adhesive for Snore and Body Position sensor (a package of 12 units)
- Cable for Tamper-Proof Bracelet
- Tamper-Proof Bracelet (a box of 24 bracelets)
- AC adapter
- USB cable
- Rechargeable Lithium Ion Battery
- Step-by-Step Reference Guide WP200 Unified + Itamar SBP
- Quick Reference Cards WP200 Unified
- Carrying case